

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E3524024D

Time Processed : 1:50:52

Month-Day-Year Processed : 05/19/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ17010507

<Chromatogram>

mV

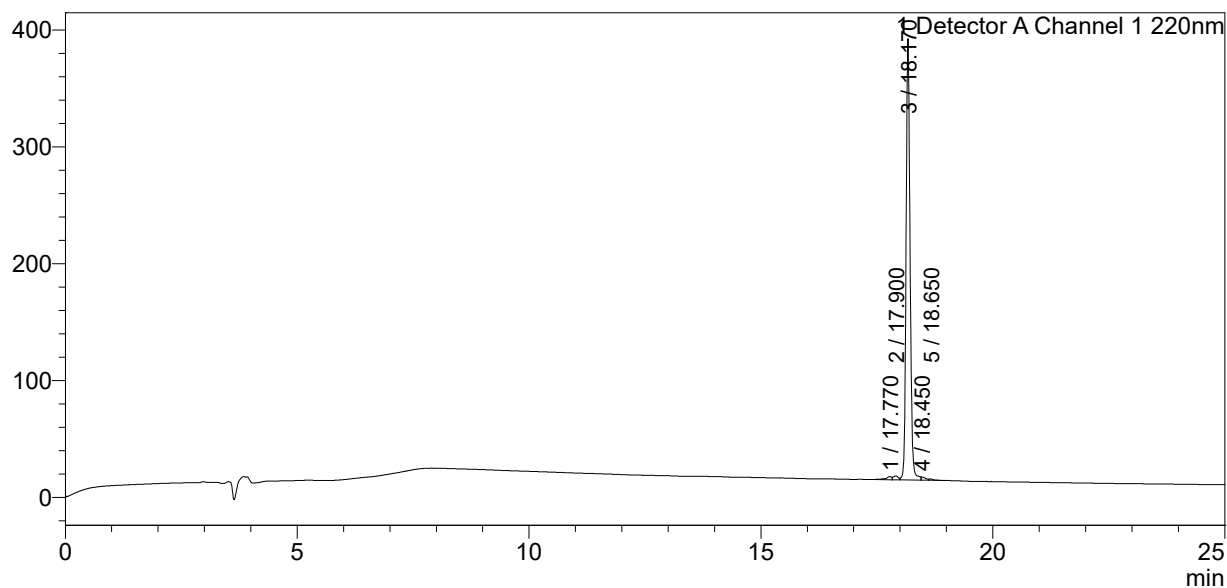

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.770	23334	2660	0.999
2	17.900	25189	3341	1.078
3	18.170	2260219	377863	96.761
4	18.450	18422	2803	0.789
5	18.650	8704	1176	0.373
Total		2335868	387843	100.000