


Mass Spectrum

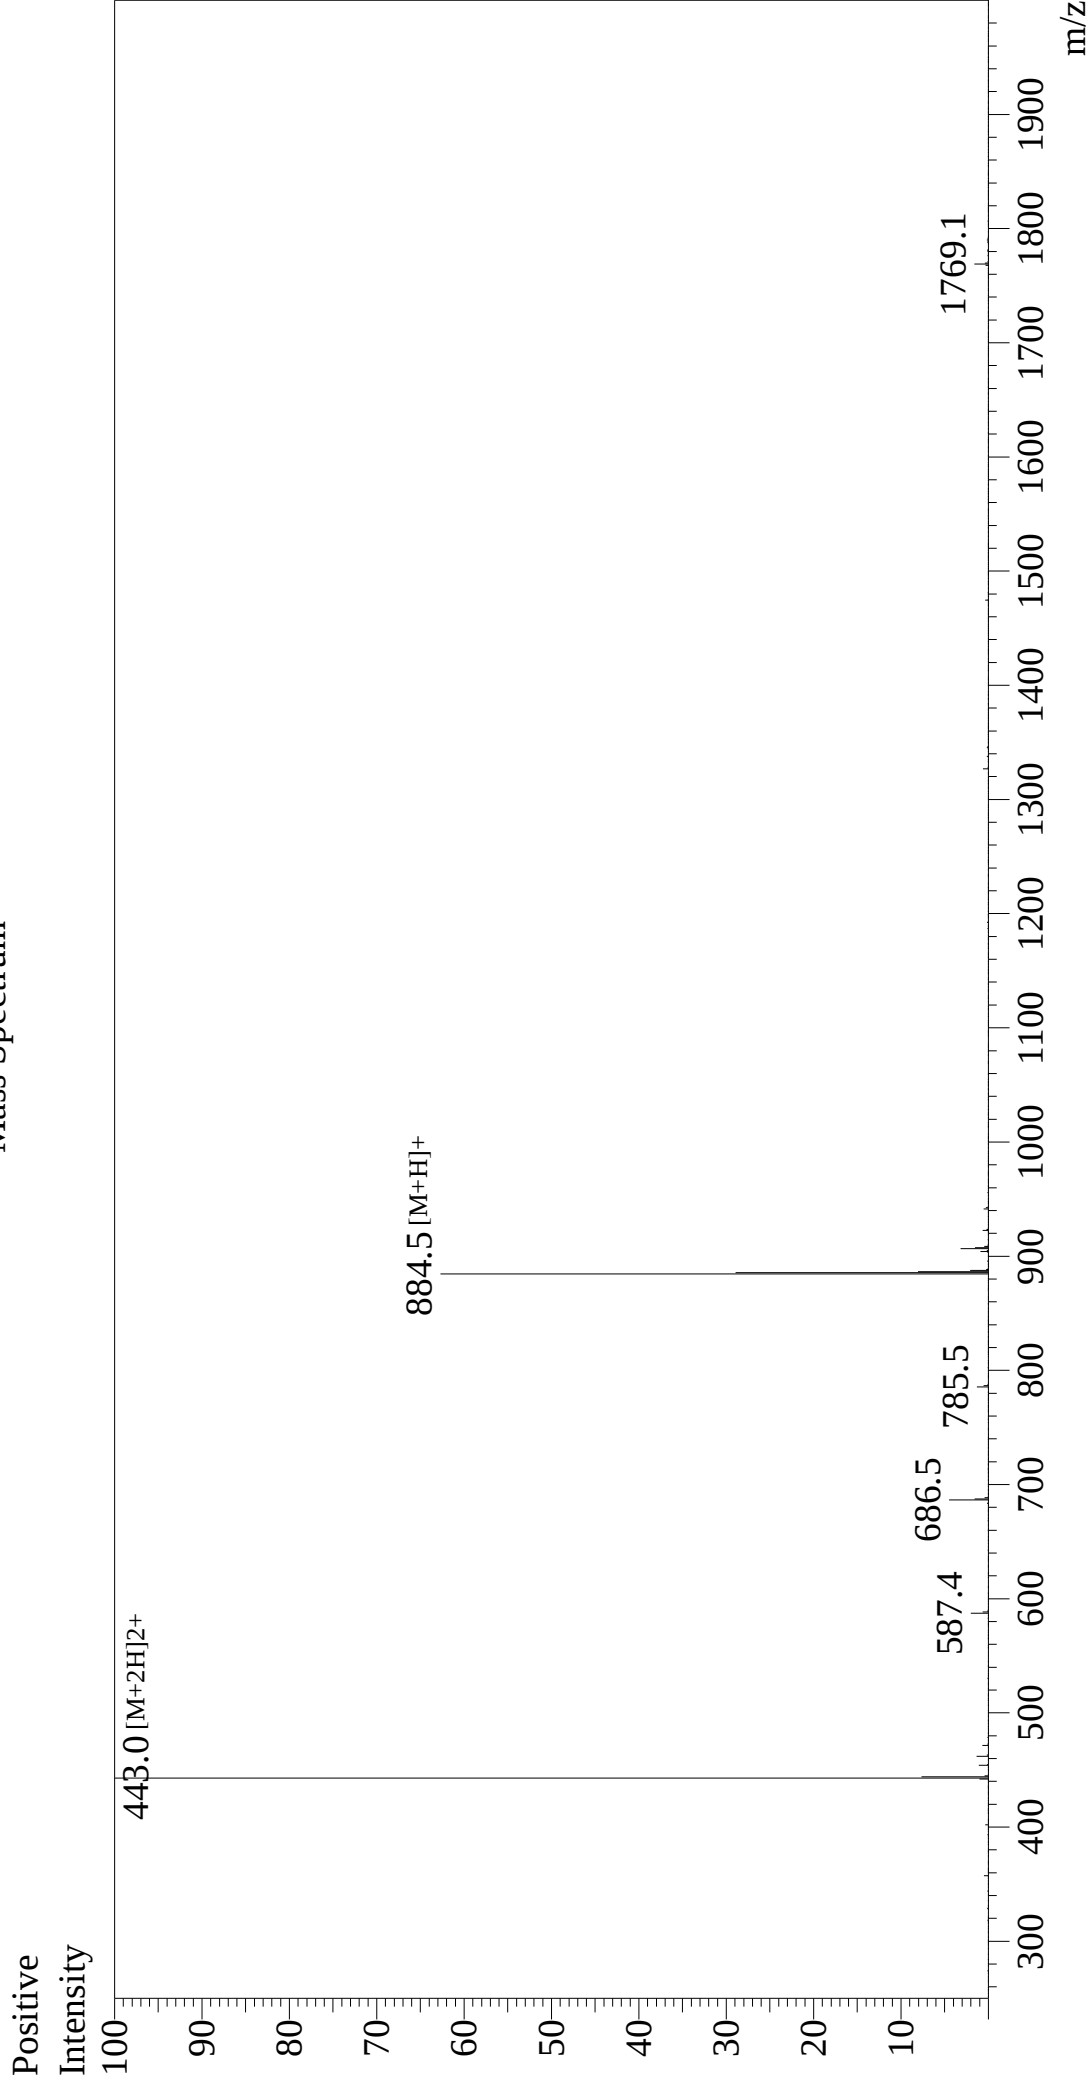

Sample Information

Month-Day Processed :	03/27/26	Interface	:ESI	Equipment	:ZJ22010150
Time Processed :	7:52:14	Nebulizing Gas Flow	:1.5L/min	Interface Bias	: +4.5 kV
Injection Volume :	0.3	CDL Temp	:250	Drying Gas Flow	:5 L/min
Sample Name :	KRAS G12V Peptide (VVVGAVGVGK)	Block Temp	:200	T.Flow	:0.2 ml/min
Cat No. : RP30229				B.conc	:50%H2O/50%MeOH
Lot No. : E3570626C					
Theoretical MW: 884.08					
Observed MW : 884.0					