

Sample Name :Biotin-β-Amyloid (1-40)

Cat No. : RP30249
Lot No. : E3571526C

Time Processed :21:01:54
Month-Day-Year Processed :04/17/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :UniPSN 30-300 30um, 4.6x250mm

<Chromatogram>

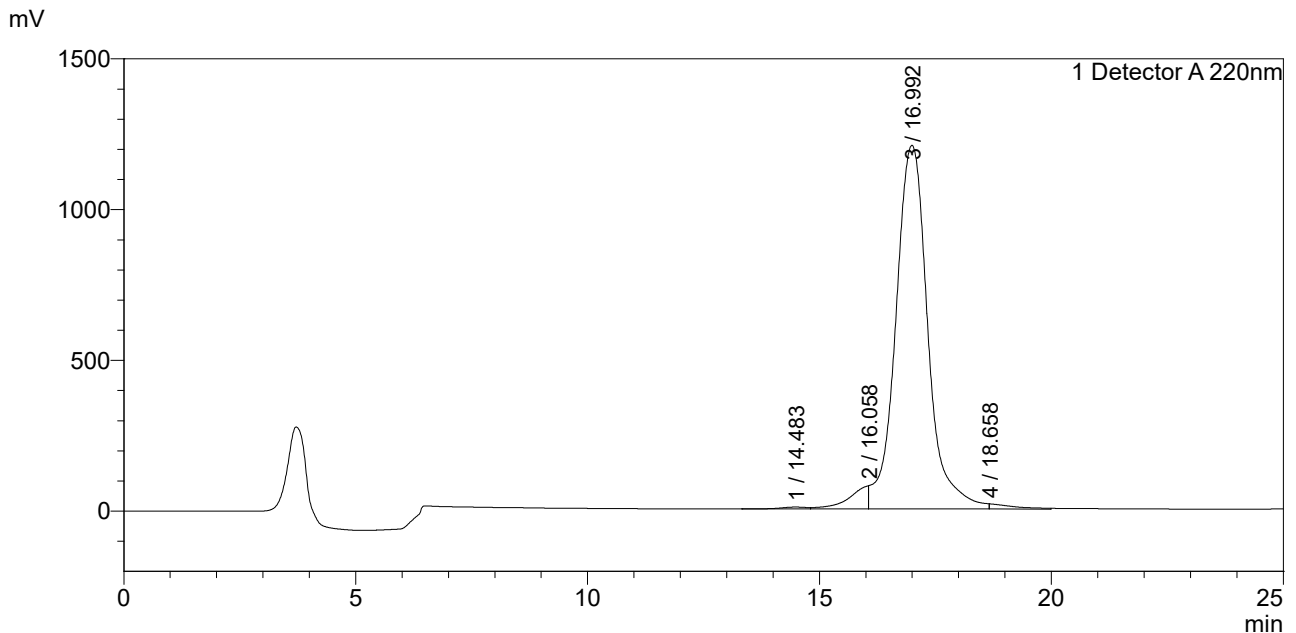

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.483	231099	6100	0.379
2	16.058	2176134	77173	3.568
3	16.992	57958690	1206407	95.041
4	18.658	617146	17320	1.012
Total		60983068	1307001	100.000