

Sample Name :IRBP (1-20), human  
Cat No. : RP20269  
Lot No. : E3590924A  
Time Processed :14:26:57  
Month-Day-Year Processed :01/05/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0310

### <Chromatogram>

mV

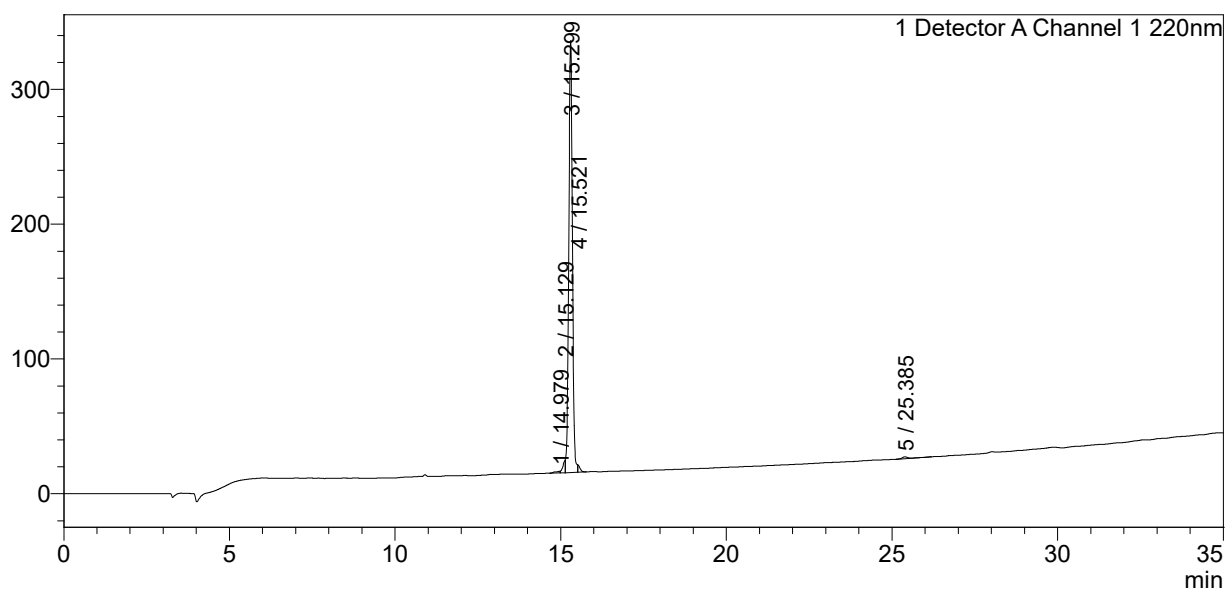

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.979	13411	1252	0.522
2	15.129	44793	8971	1.743
3	15.299	2470150	320531	96.146
4	15.521	23592	5450	0.918
5	25.385	17209	1467	0.670
Total		2569156	337671	100.000