

Sample Name:IRBP (1-20), human
Cat No. : RP20269
Lot No. : E3637123E
Time Processed :11:45:47
Month-Day-Year Processed :06/16/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: GR11010440

<Chromatogram>

mV

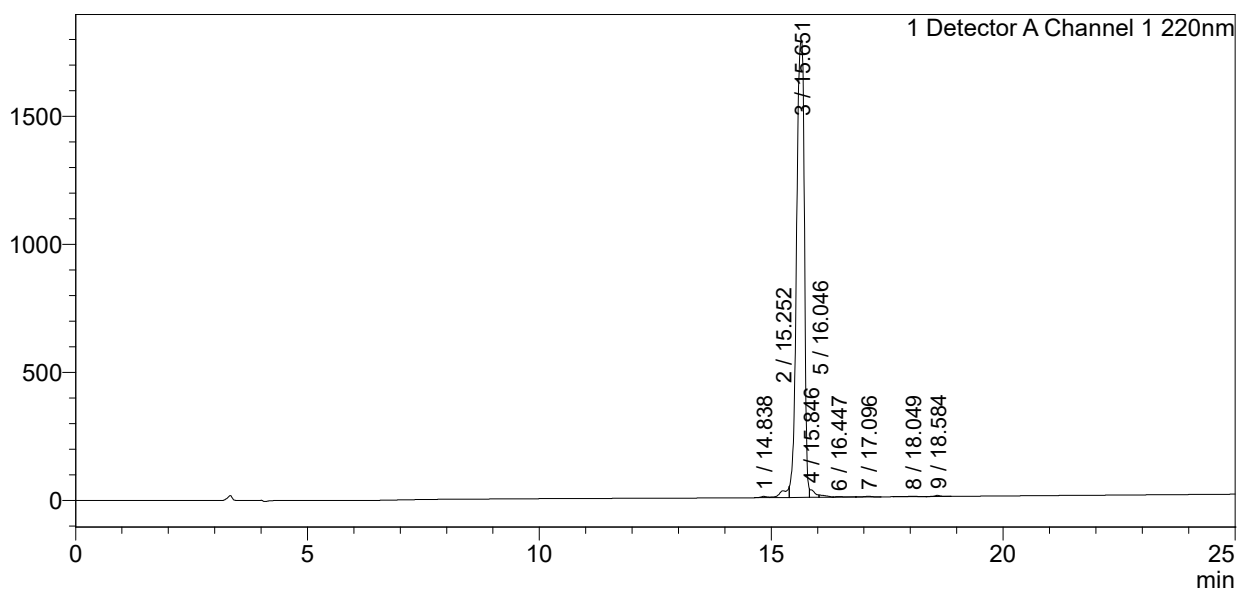

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.838	47674	4966	0.221
2	15.252	406404	26542	1.884
3	15.651	20678058	1784550	95.842
4	15.846	236700	29387	1.097
5	16.046	90032	8835	0.417
6	16.447	33719	1820	0.156
7	17.096	31266	2788	0.145
8	18.049	19226	1744	0.089
9	18.584	32036	3873	0.148
Total		21575115	1864504	100.000