

Sample Name : Biotin- β -Amyloid (1-40)
 Cat No. : RP30249
 Lot No. : E3641526A
 Time Processed : 15:17:29
 Month-Day-Year Processed : 02/01/2026
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : UniPSN 30-300 30um, 4.6x250mm

<Chromatogram>

mV

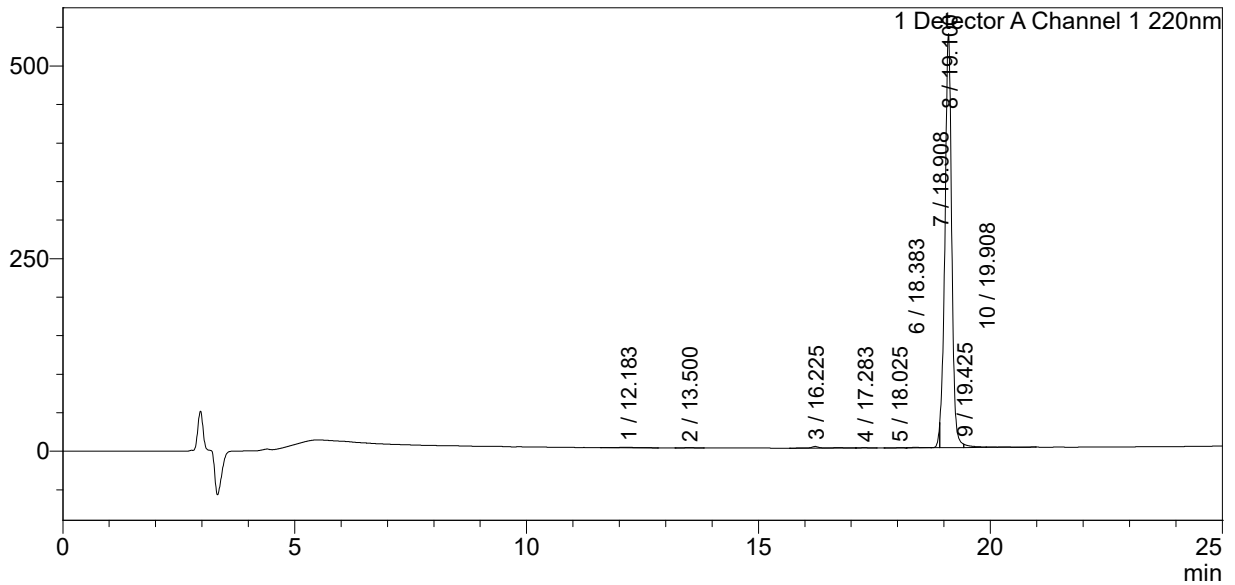

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.183	17023	559	0.302
2	13.500	6328	446	0.112
3	16.225	34699	2127	0.615
4	17.283	3840	364	0.068
5	18.025	3715	302	0.066
6	18.383	9629	789	0.171
7	18.908	63391	32387	1.124
8	19.100	5446820	537406	96.545
9	19.425	45954	4383	0.815
10	19.908	10319	583	0.183
Total		5641717	579347	100.000