

Sample Name :RGD  
 Cat No. :RP20297  
 Lot No. :E3746426C  
 Time Processed :19:43:47  
 Month-Day-Year Processed :03/21/2026  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm  
 Equipment: ZJ25010053

### <Chromatogram>

mV

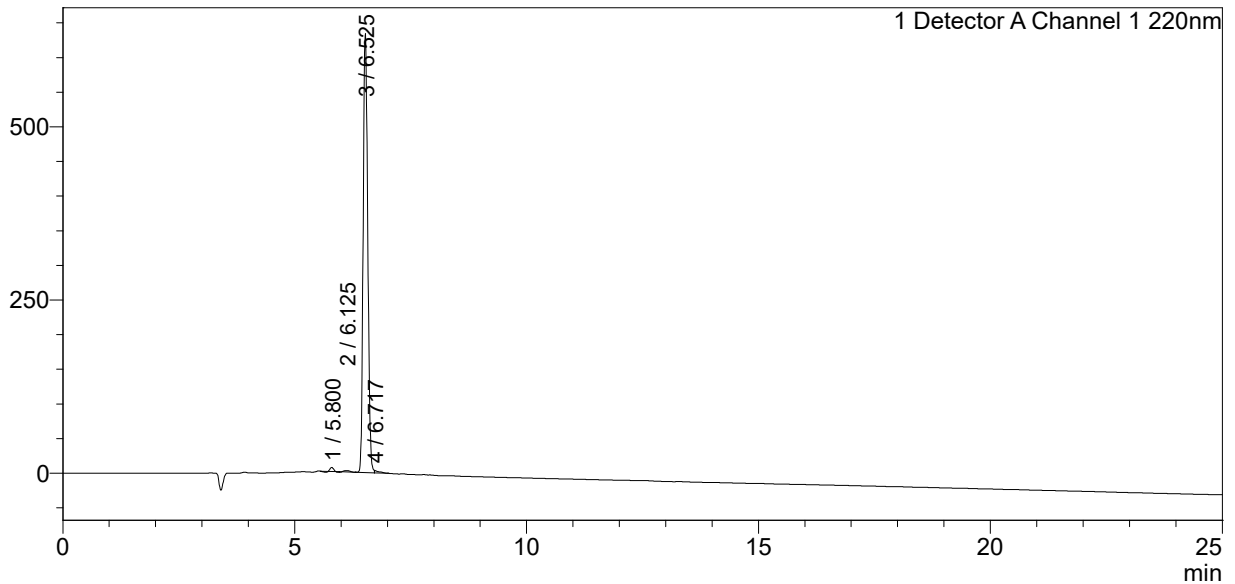

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.800	20897	5888	0.475
2	6.125	15145	1925	0.344
3	6.525	4339668	633621	98.649
4	6.717	23409	3742	0.532
Total		4399119	645176	100.000