


Mass Spectrum

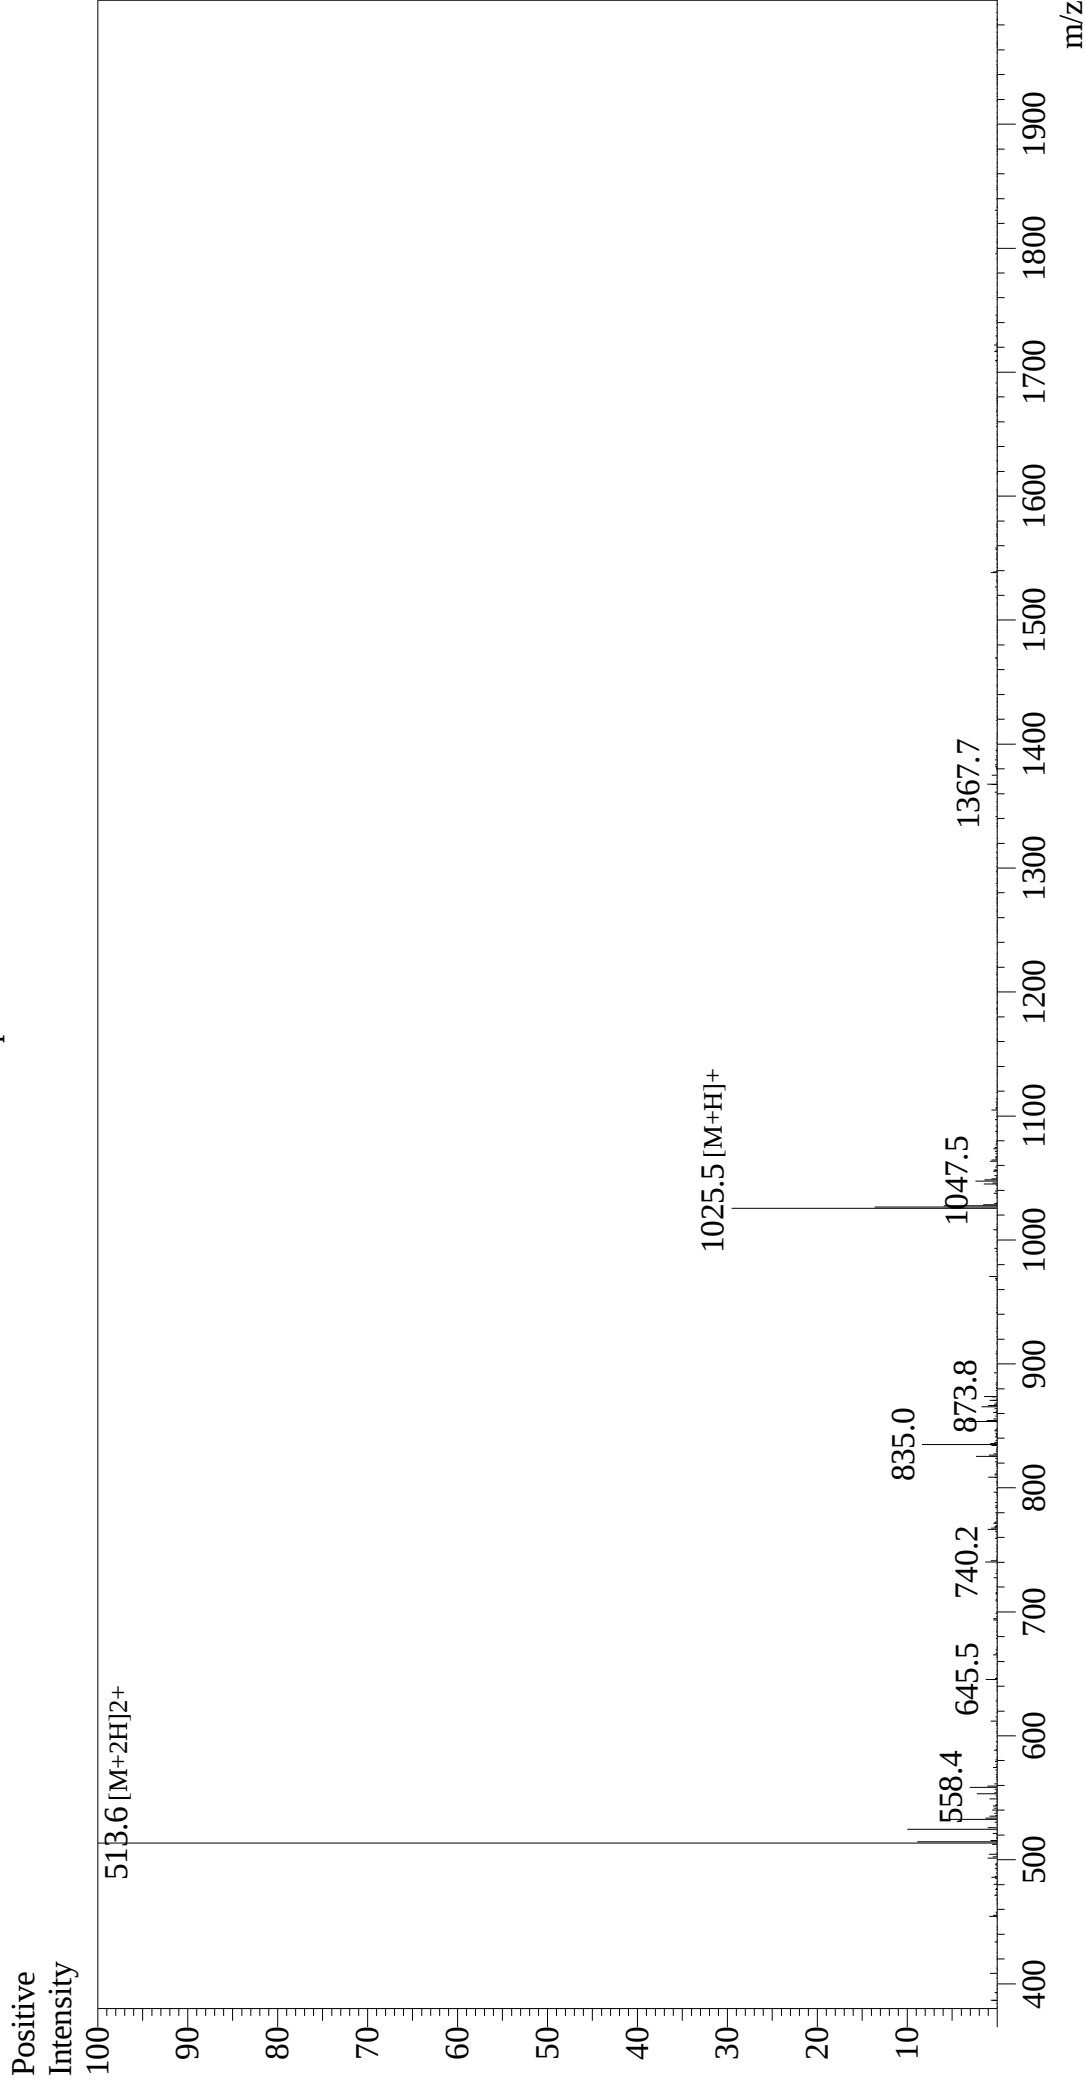

Sample Information

Month-Day Processed : 03/22/26

Time Processed : 8:04:48

Injection Volume : 0.3

Sample Name : RGD

Cat No. : RP20297

Lot No. : E3746426C

Theoretical MW : 1025.06

Observed MW : 1025.2

Interface

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Interface Bias

Drying Gas Flow

T.Flow

B.conc

:ZJ22010150

: +4.5 kV

:5 L/min

:0.2 ml/min

:50%H₂O/50%MeOH