

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E3817325C
Time Processed :15:34:36
Month-Day-Year Processed :04/07/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010142

<Chromatogram>

mV

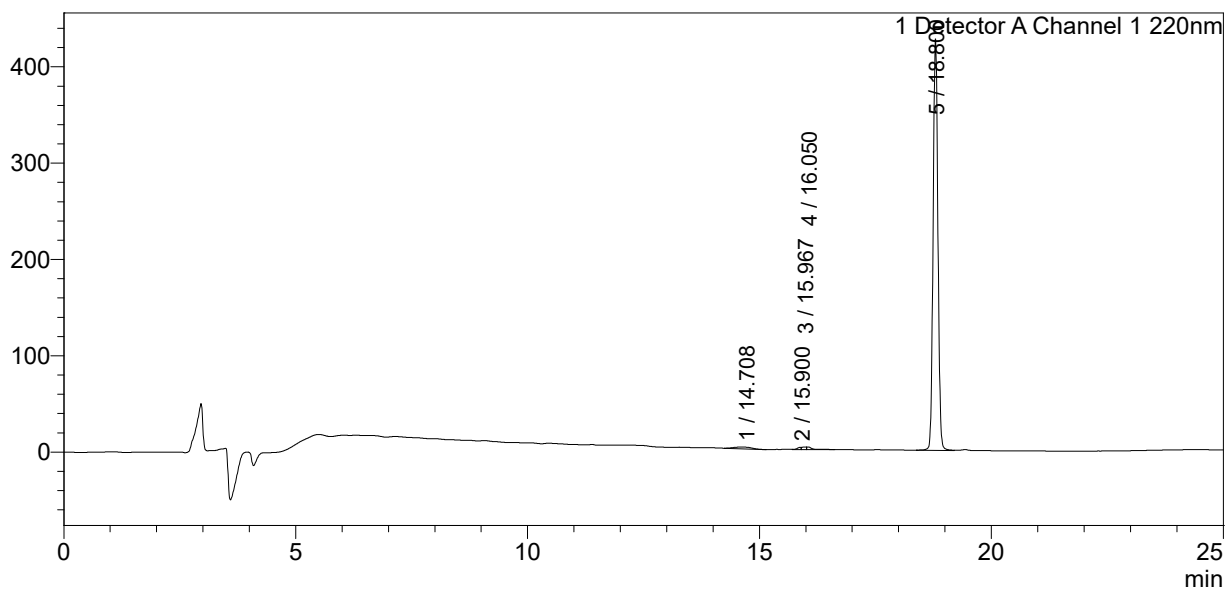

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.708	49733	1853	1.557
2	15.900	14718	2413	0.461
3	15.967	18391	2780	0.576
4	16.050	24358	2771	0.762
5	18.800	3087526	427339	96.644
Total		3194727	437157	100.000