

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E3817824A
Time Processed :17:05:58
Month-Day-Year Processed :01/21/2024
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ19010014

<Chromatogram>

mV

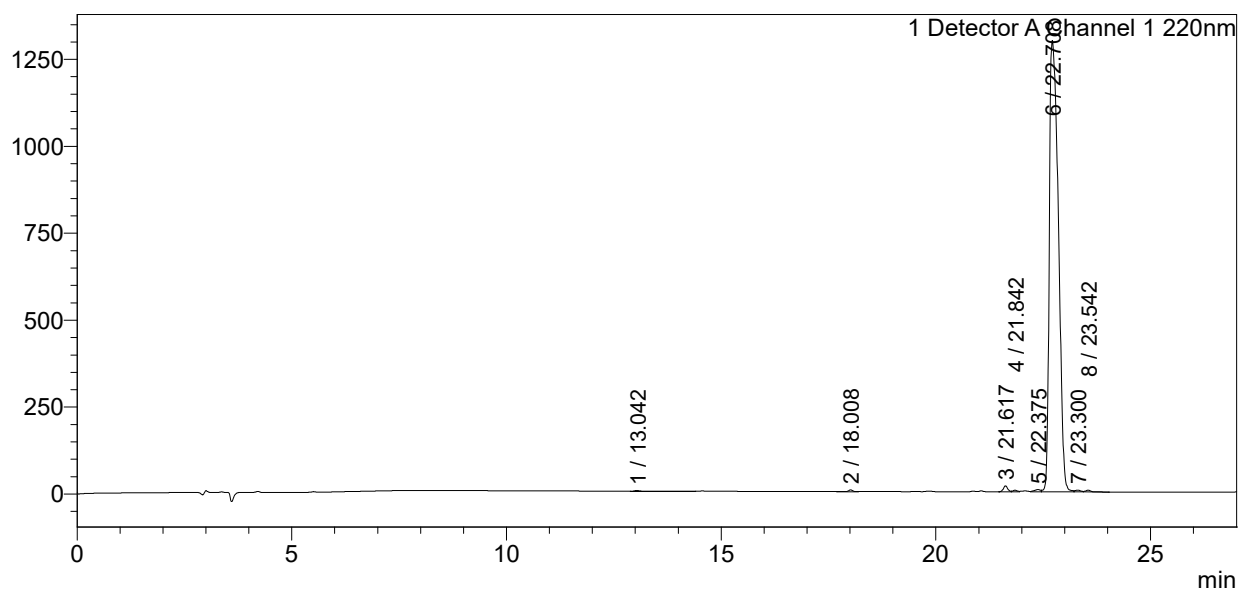

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.042	115252	3055	0.595
2	18.008	40108	5099	0.207
3	21.617	118546	16858	0.612
4	21.842	31078	4378	0.160
5	22.375	65635	6652	0.339
6	22.708	18901570	1298501	97.611
7	23.300	48200	5398	0.249
8	23.542	43737	5356	0.226
Total		19364126	1345297	100.000