


Mass Spectrum

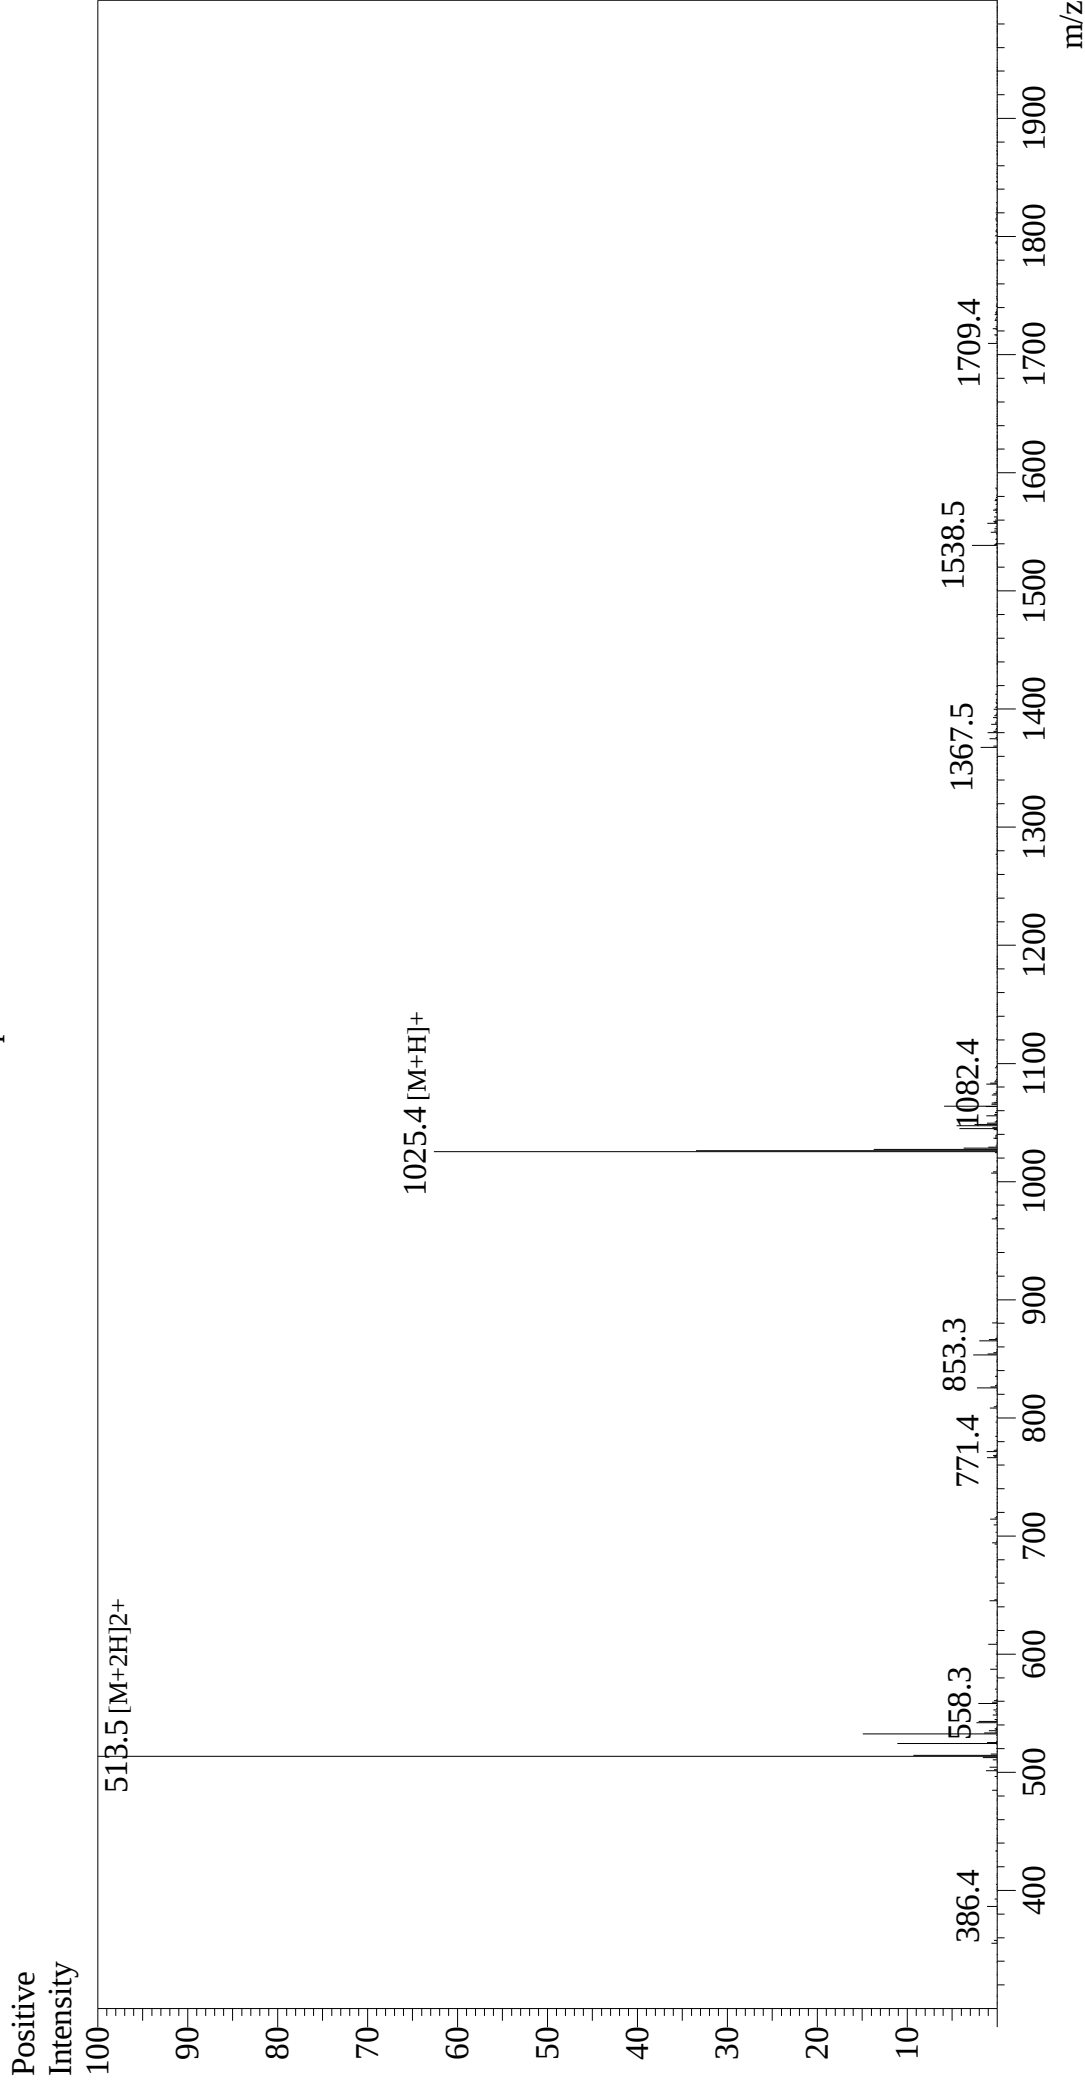

Sample Information

Month-Day Processed : 08/15/23
 Time Processed : 20:31:39
 Injection Volume : 0.2
 Sample Name : RGD
 Cat No. : RP20297
 Lot No. : E3901823H
 Theoretical MW : 1025.06
 Observed MW : 1025.0

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : ZJ22010150
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O / 50% MeOH