

Sample Name :IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E3906325A
 Time Processed :15:49:20
 Month-Day-Year Processed :02/10/2025
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ20010140

<Chromatogram>

mV

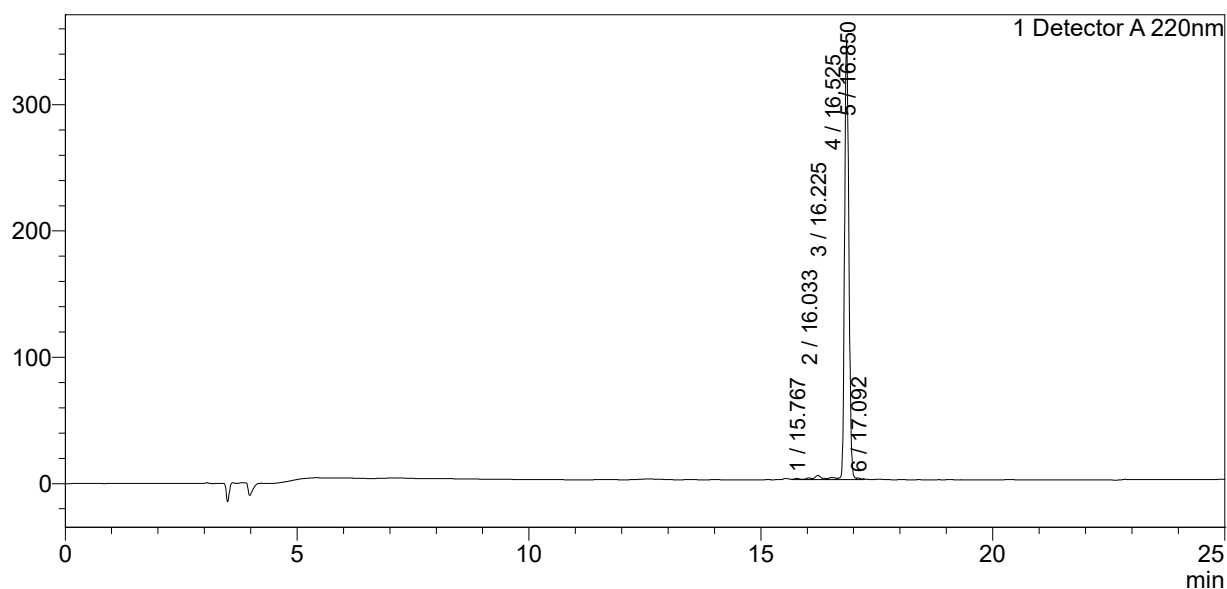

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.767	8354	1034	0.363
2	16.033	11614	1464	0.505
3	16.225	34283	3367	1.492
4	16.525	17813	1711	0.775
5	16.850	2217889	347651	96.497
6	17.092	8442	1206	0.367
Total		2298395	356433	100.000