

Sample Name : β -Endorphin, human
 Cat No. : RP11344
 Lot No. : E3938922I
 Time Processed :21:02:20
 Month-Day-Year Processed :10/03/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: GK11010009

<Chromatogram>

mV

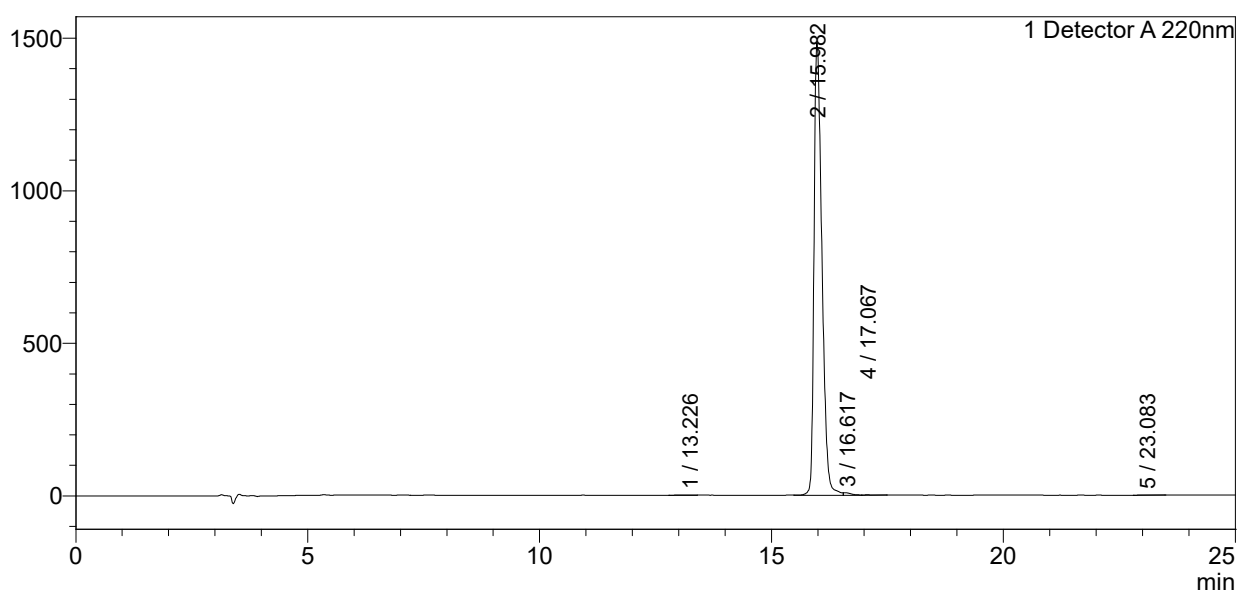

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.226	24869	1260	0.140
2	15.982	17612815	1482051	99.154
3	16.617	93852	7698	0.528
4	17.067	23415	1134	0.132
5	23.083	8198	372	0.046
Total		17763149	1492515	100.000