

Sample Name :IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E3995025B

Time Processed :19:34:53

Month-Day-Year Processed :02/23/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ19010141

<Chromatogram>

mV

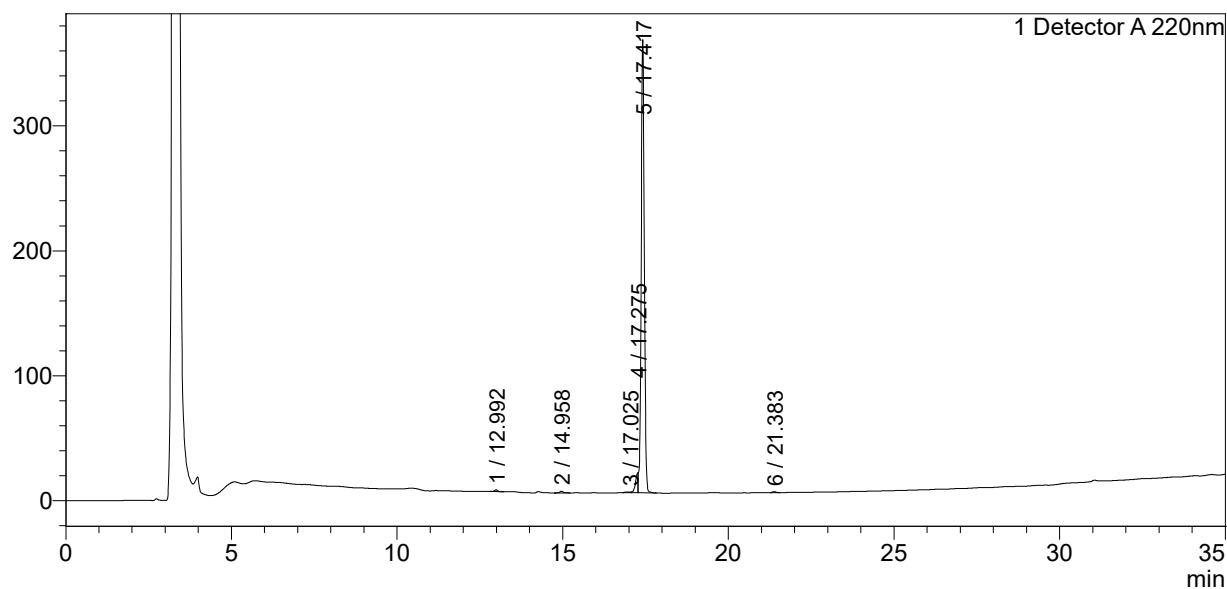

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.992	8879	1395	0.357
2	14.958	11046	1364	0.444
3	17.025	6561	602	0.264
4	17.275	82488	15932	3.318
5	17.417	2371936	362716	95.407
6	21.383	5224	783	0.210
Total		2486134	382792	100.000