


Mass Spectrum

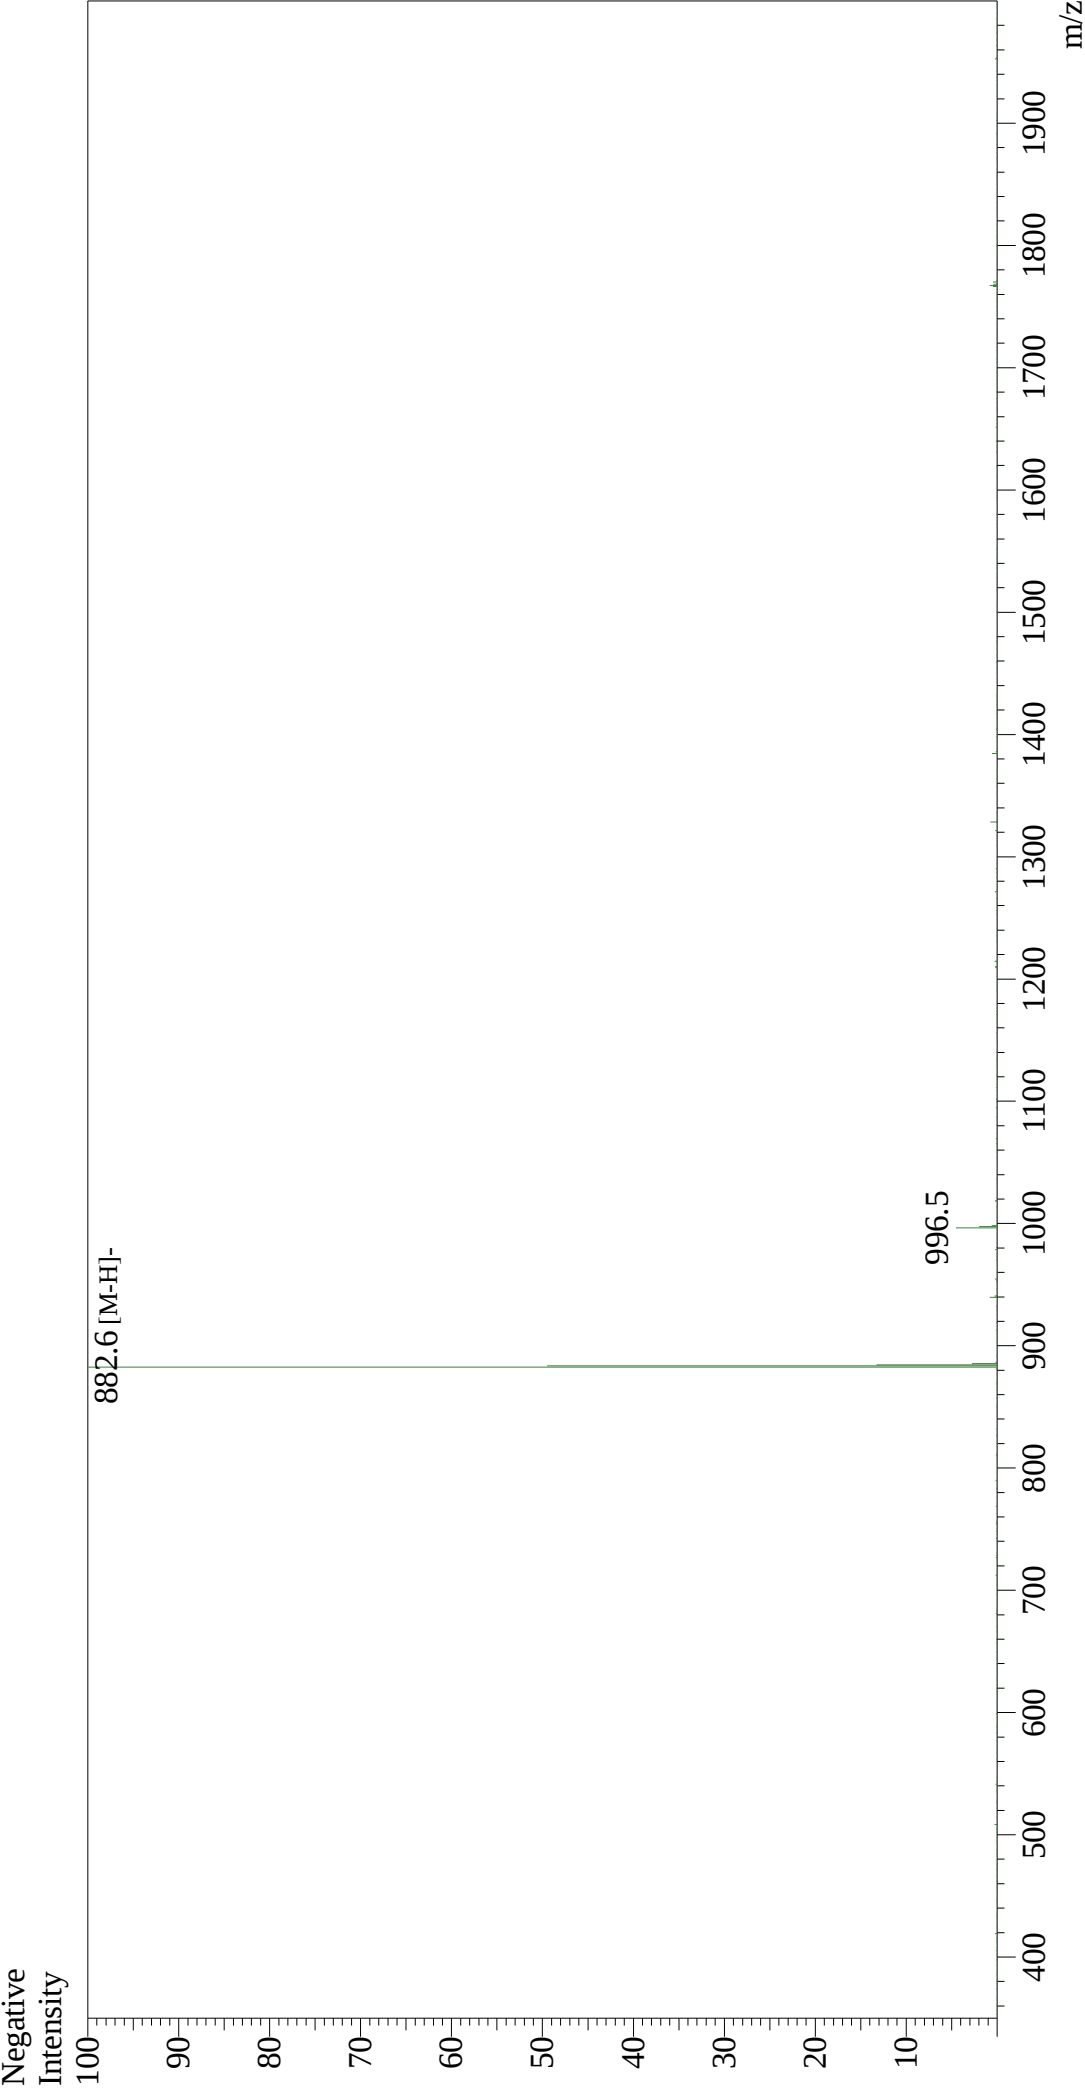

Sample Information

Month-Day Processed : 05/15/26  
Time Processed : 16:29:11  
Injection Volume : 0.3  
Sample Name : KRAS G12V Peptide (VVVGAVGVGK)  
Cat No. : RP30229  
Lot No. : E4068226E  
Theoretical MW: 884.08  
Observed MW : 883.6

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200  
Equipment : ZJ21010035  
Interface Bias : -3.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H2O/50%MeOH