


Mass Spectrum

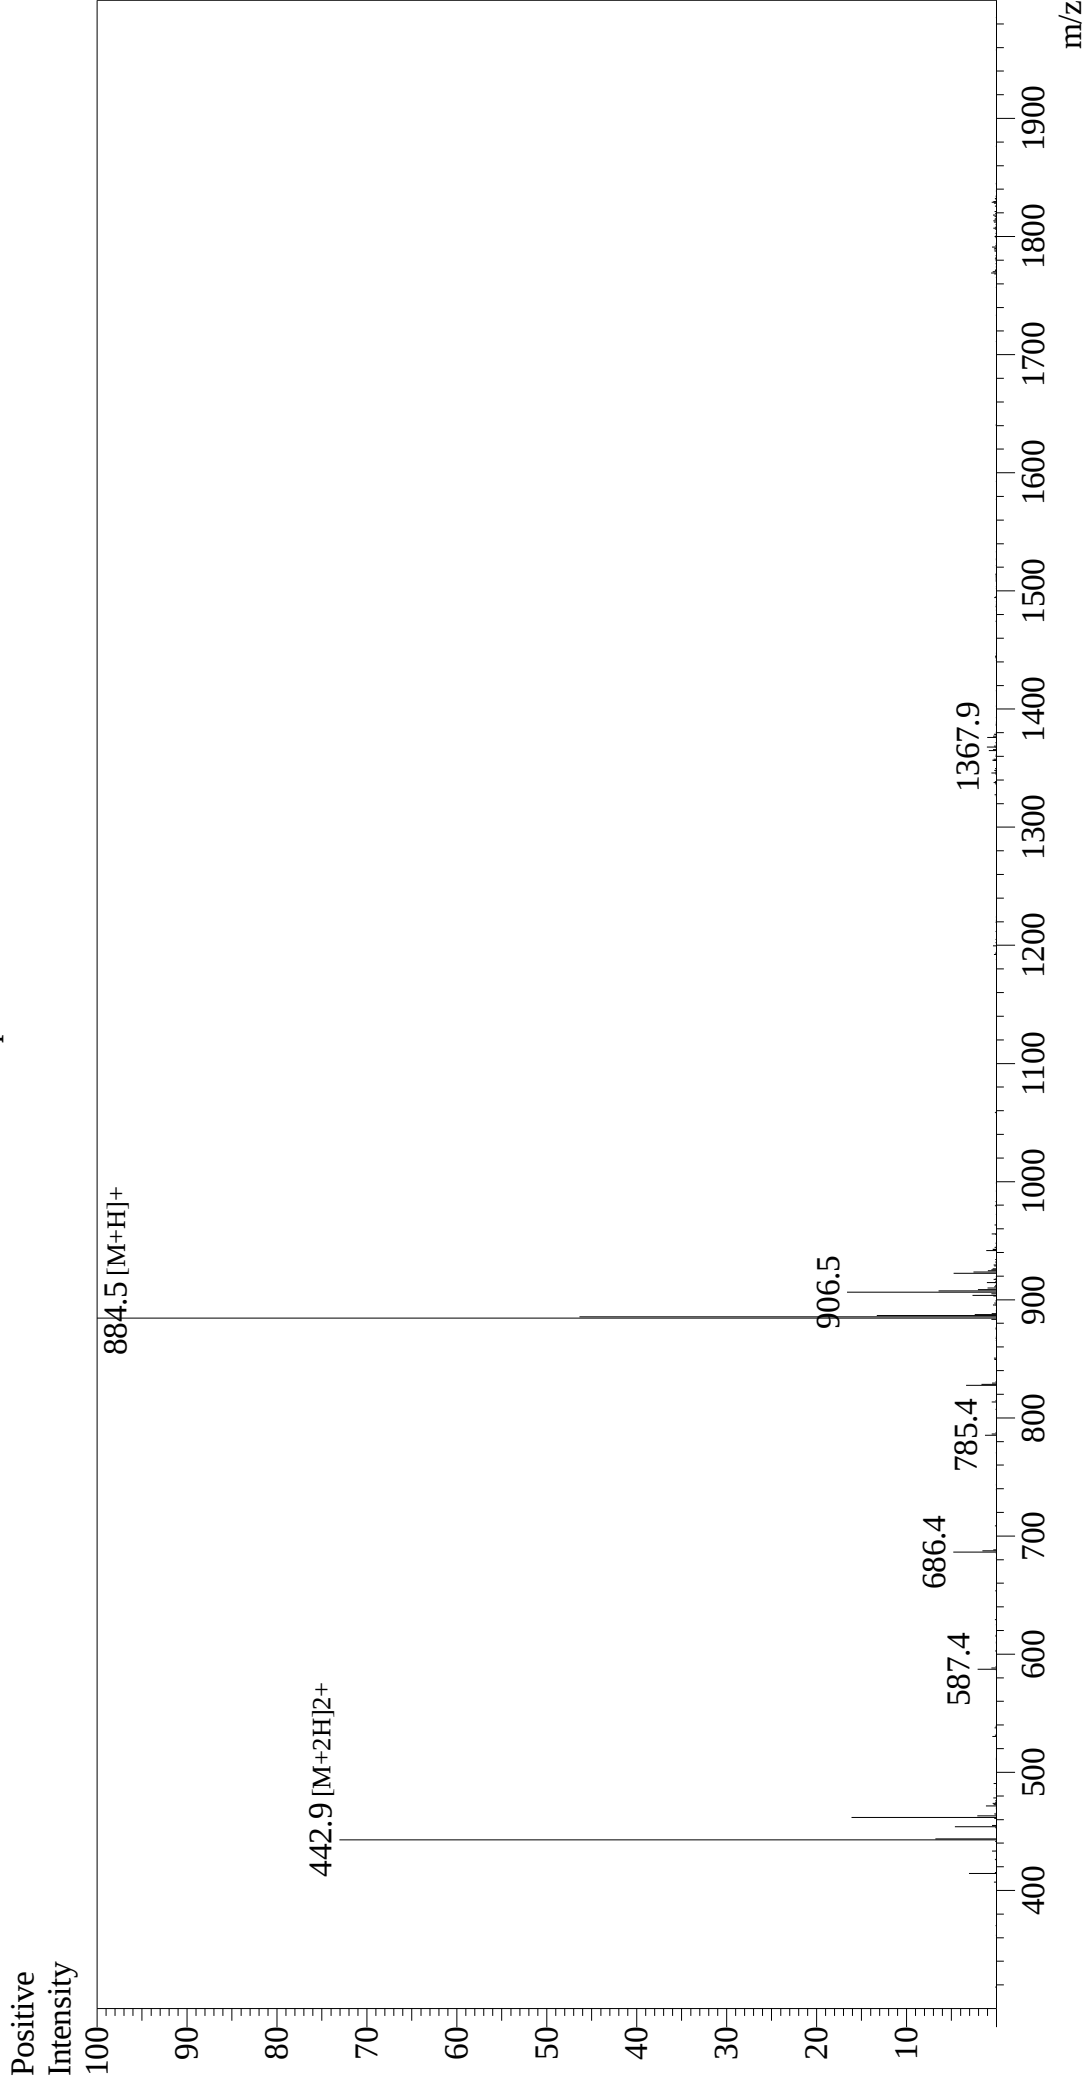

Sample Information

Month-Day Processed : 03/03/24

Time Processed : 21:35:48

Injection Volume : 0.6

Sample Name : KRAS G12V Peptide (VVVGAVGVGK)

Cat No. : RP30229

Lot No. : E4083124B

Theoretical MW : 884.08

Observed MW : 883.5

Interface : ESI

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment : ZJ21010035

Interface Bias : +4.5 kV

Drying Gas Flow : 5 L/min

T.Flow : 0.2 ml/min

B.conc : 50% H₂O/50% MeOH