


Mass Spectrum

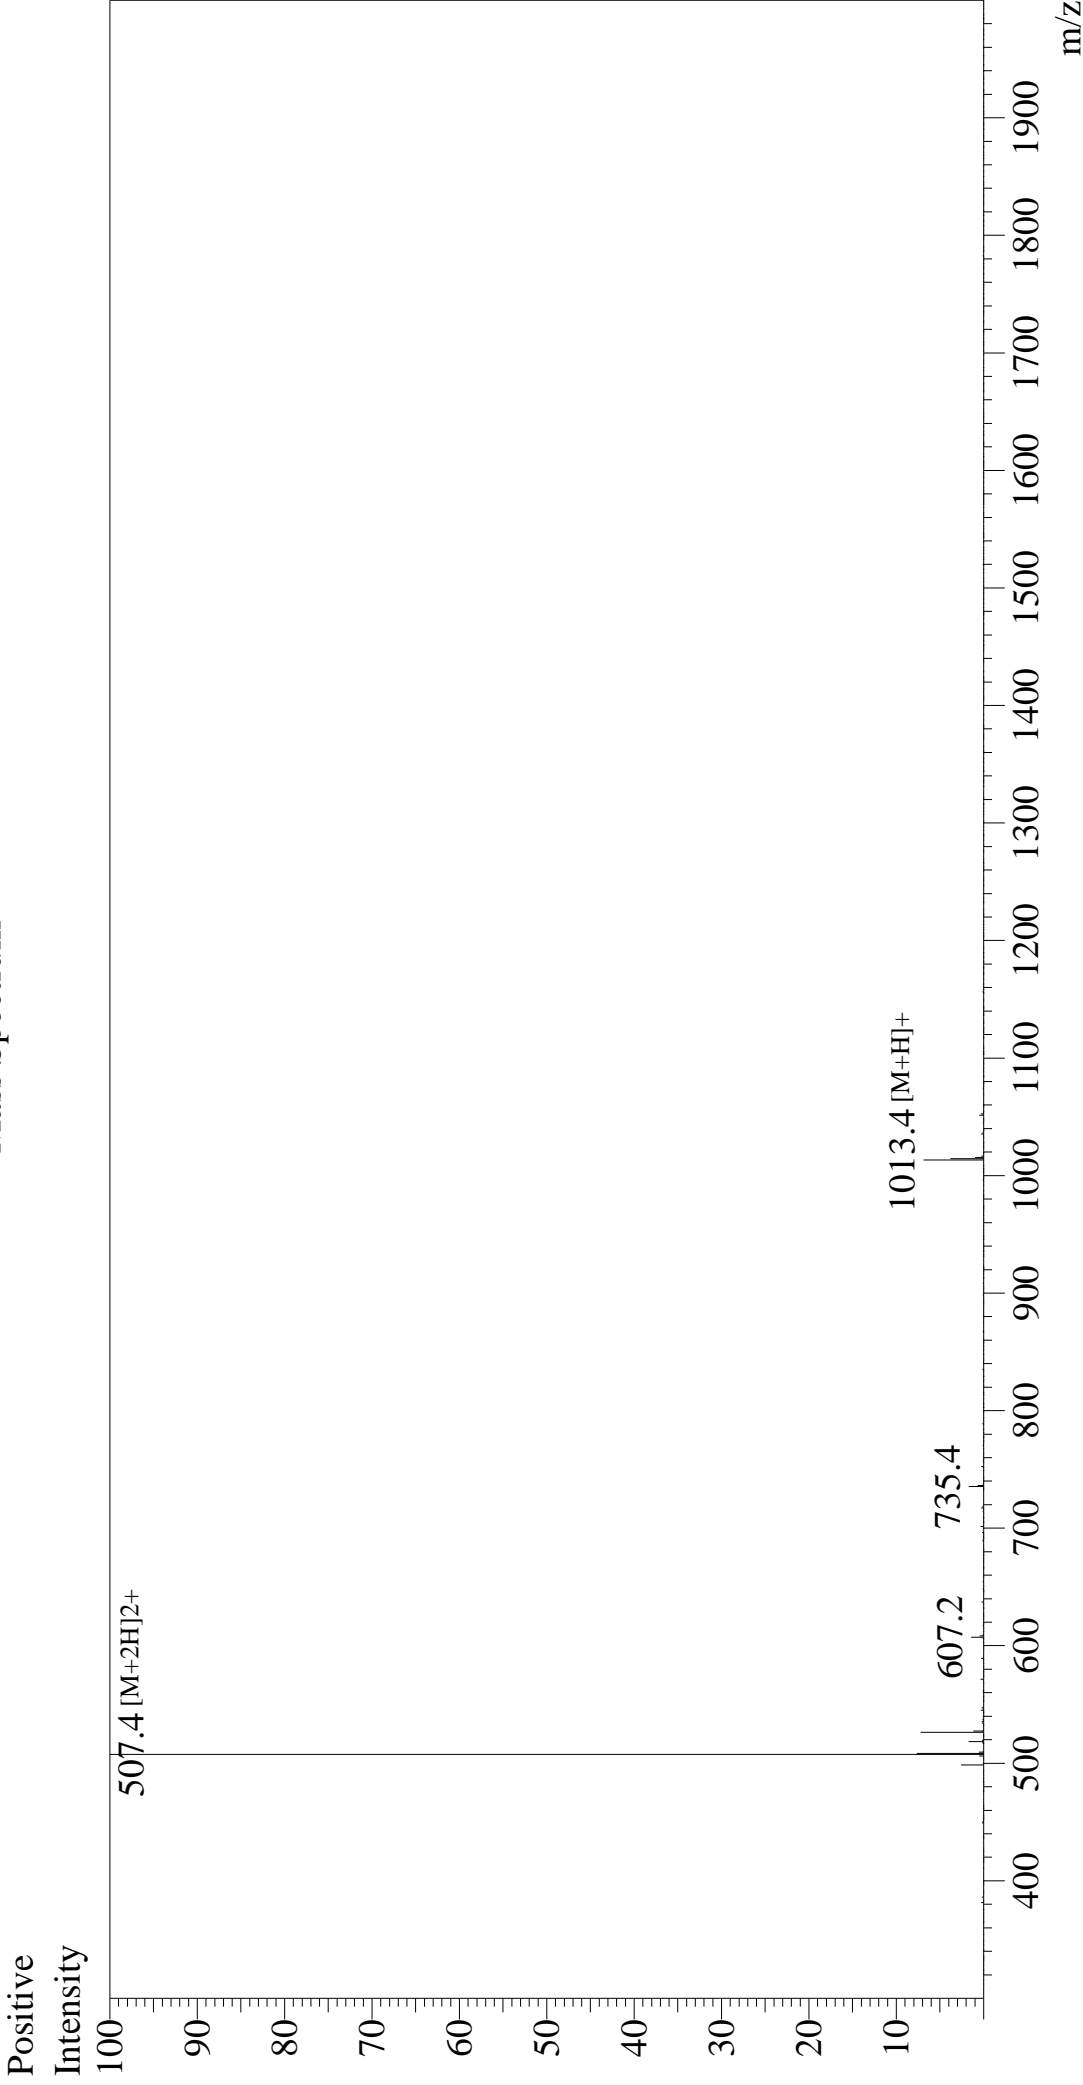

Sample Information

Month-Day Processed :	02/27/24	Equipment :	ZI21010035
Time Processed :	12:28:11	Interface Bias :	+4.5 kV
Injection Volume :	0.4	Drying Gas Flow :	5 L/min
Sample Name :	DYKDDDDK Peptide	T.Flow :	0.2 ml/min
Cat No. :	RP10586	B.conc :	50%H2O/50%MeOH
Lot No. :	E4094024B		
Theoretical MW:	1012.97		
Observed MW :	1012.8		