


Mass Spectrum

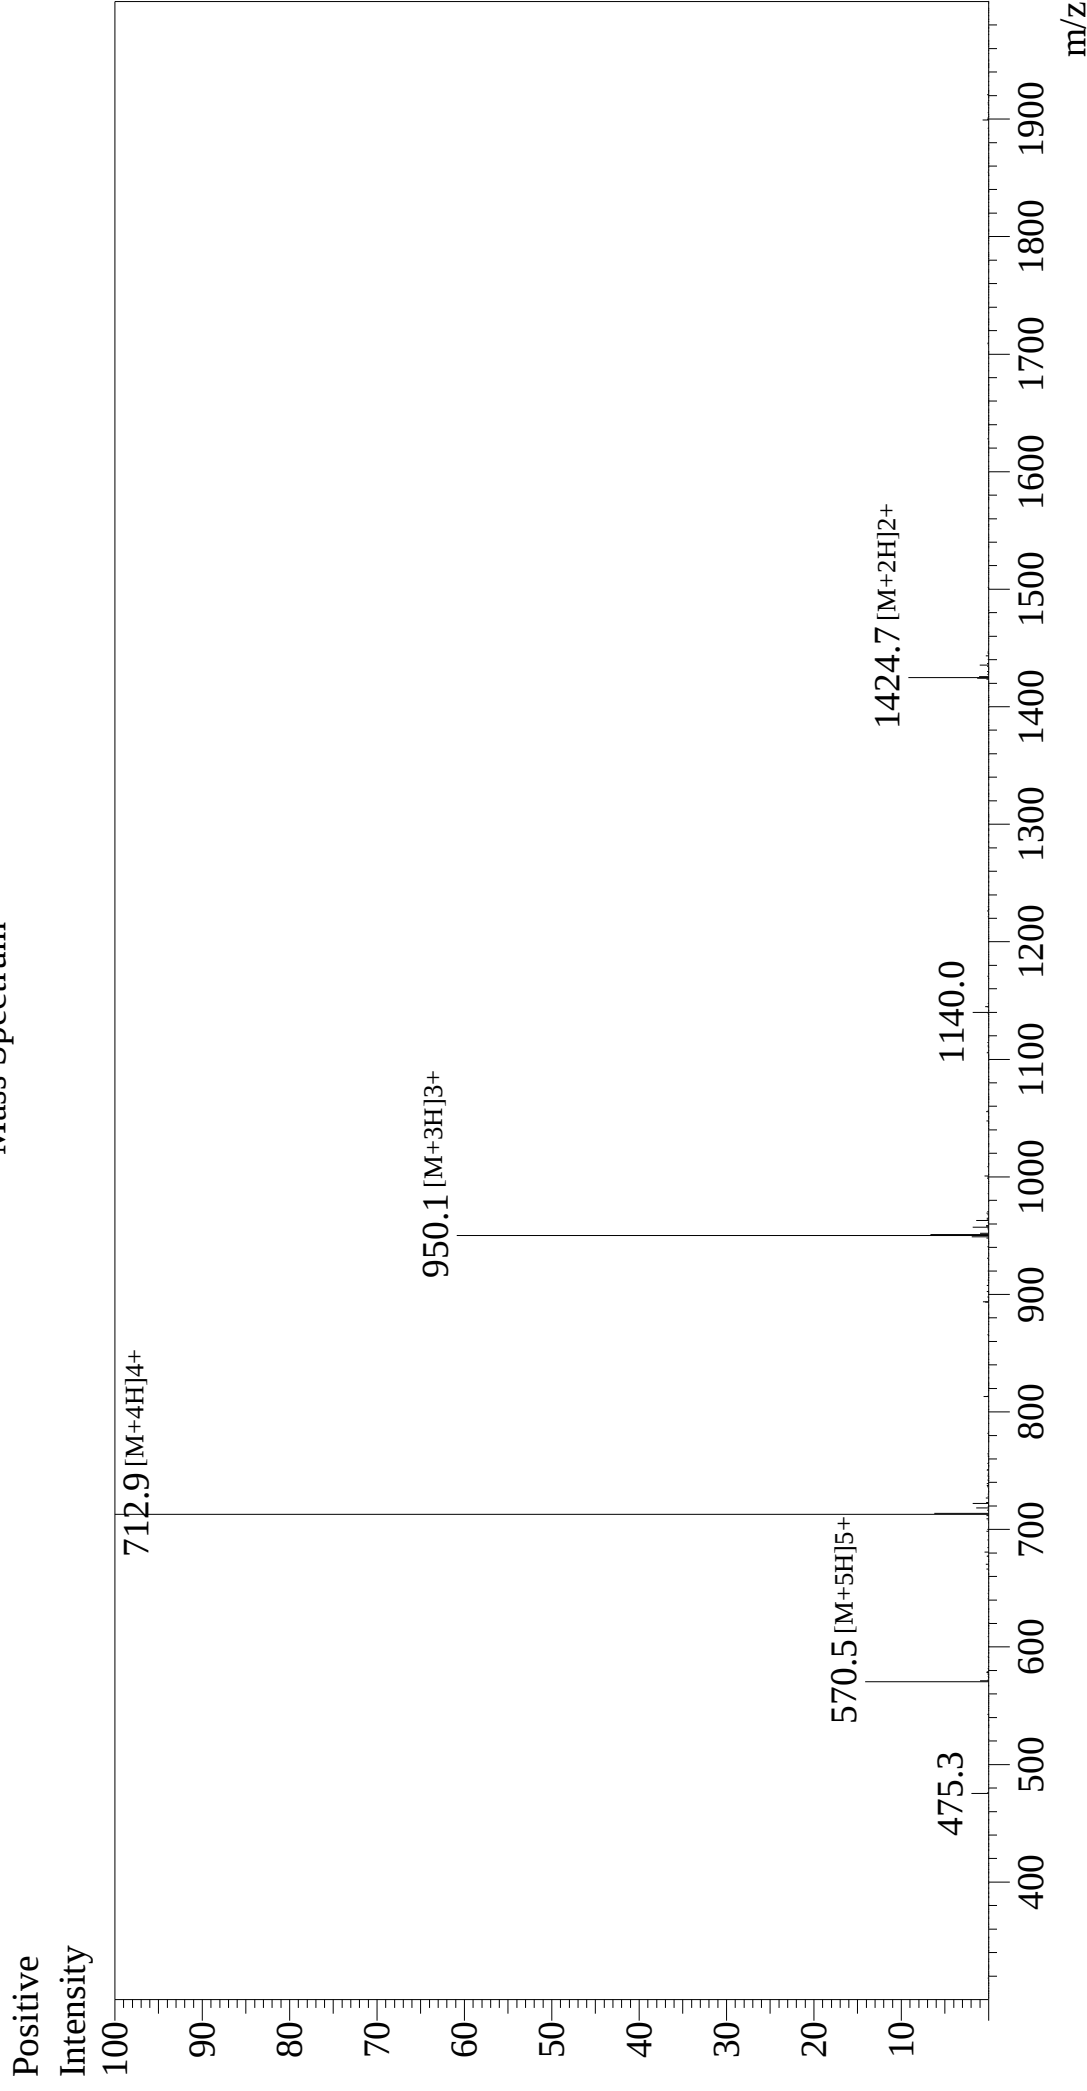

Sample Information

Month-Day Processed : 12/08/24
Time Processed : 17:15:04
Injection Volume : 0.2
Sample Name : Melittin,honey bee
Cat No. : RP20415
Lot No. : E4129324L
Theoretical MW : 2847.50
Observed MW : 2847.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeC