


Mass Spectrum

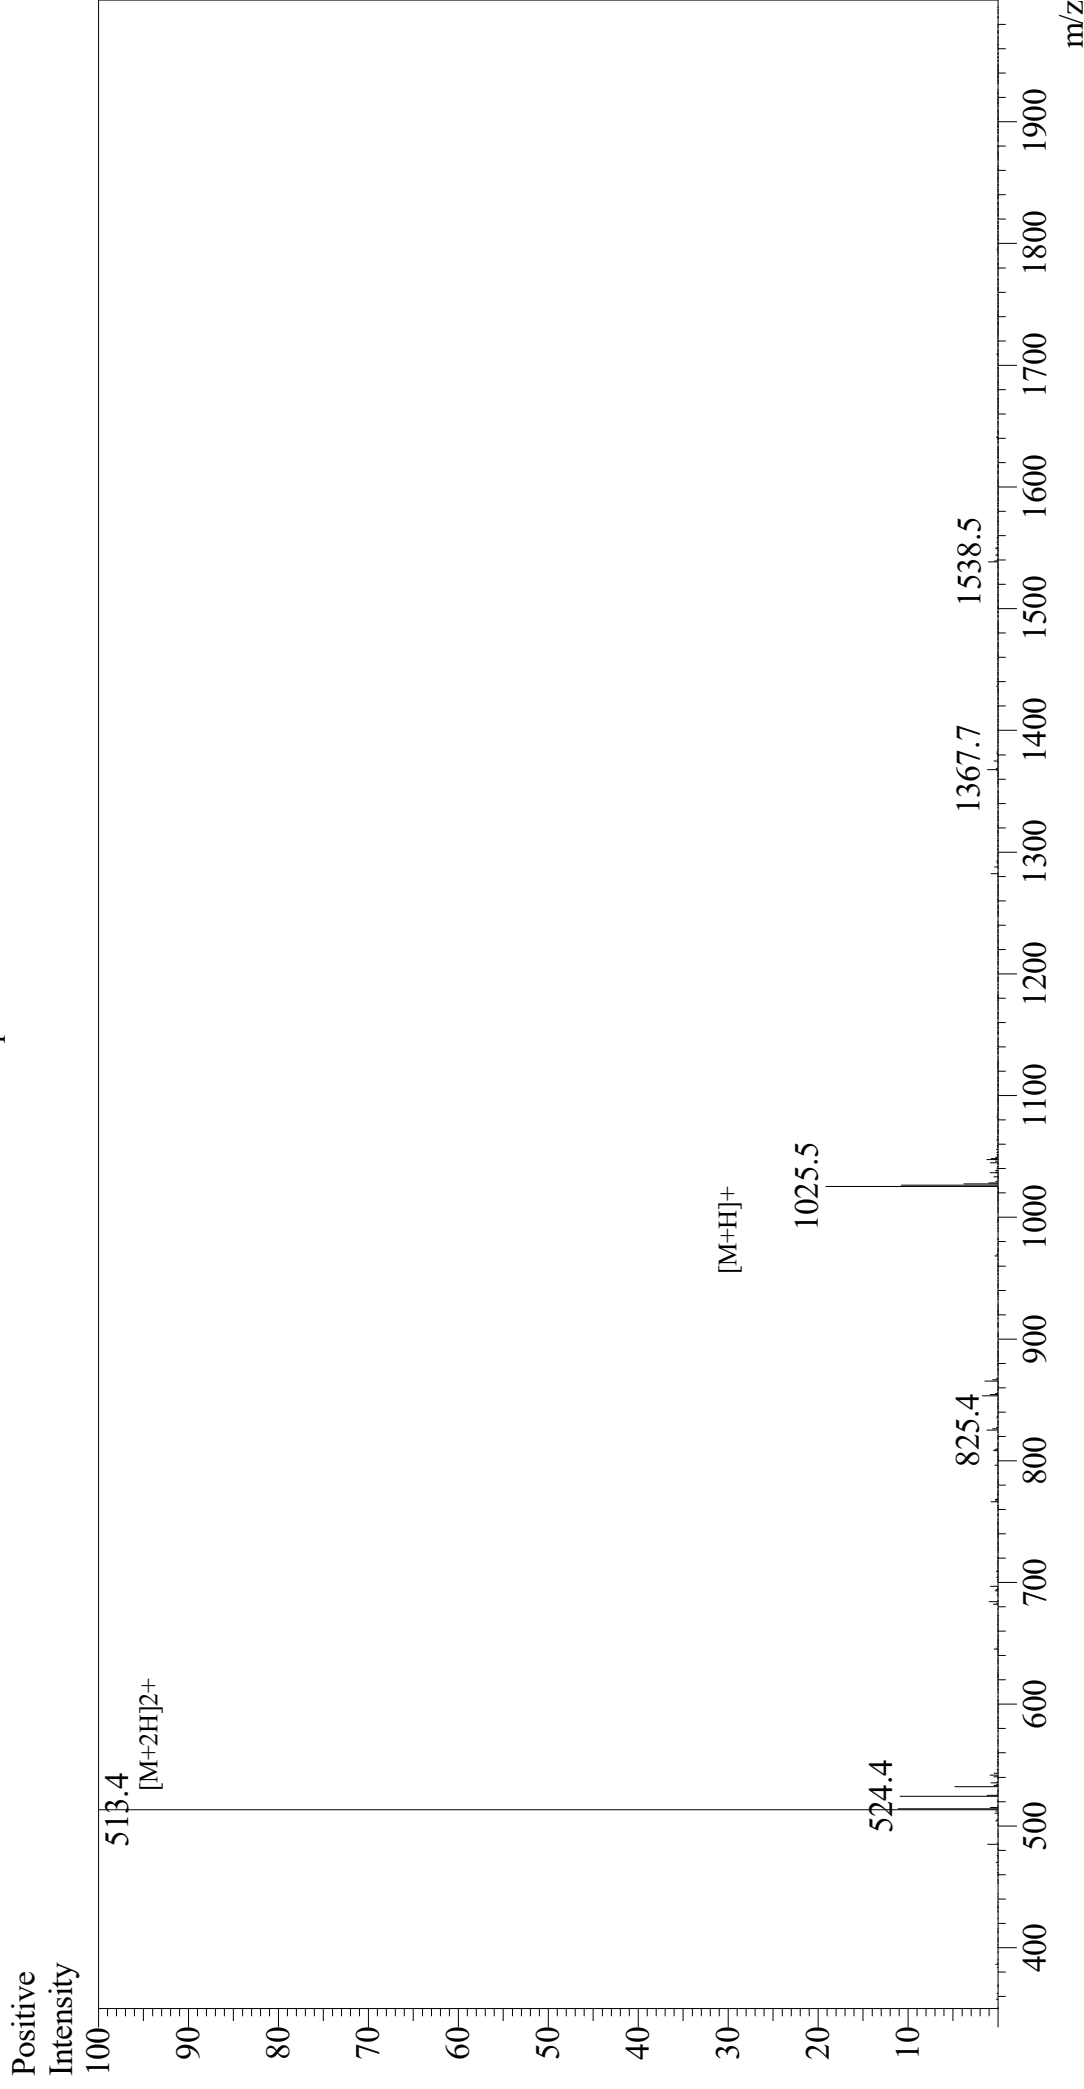

Sample Information

Month-Day Processed : 03/09/22
 Time Processed : 1:17:31 PM
 Injection Volume : 0.2
 Sample Name : RGD
 Cat No. : RP20297
 Lot No. : E4143122B
 Theoretical MW : 1025.06
 Observed MW : 1024.8

Interface : ESI
 Nebulizing Gas Flow : 1.5 L/min
 CDL Temp : 250
 Block Temp : 200
 Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH