


Mass Spectrum

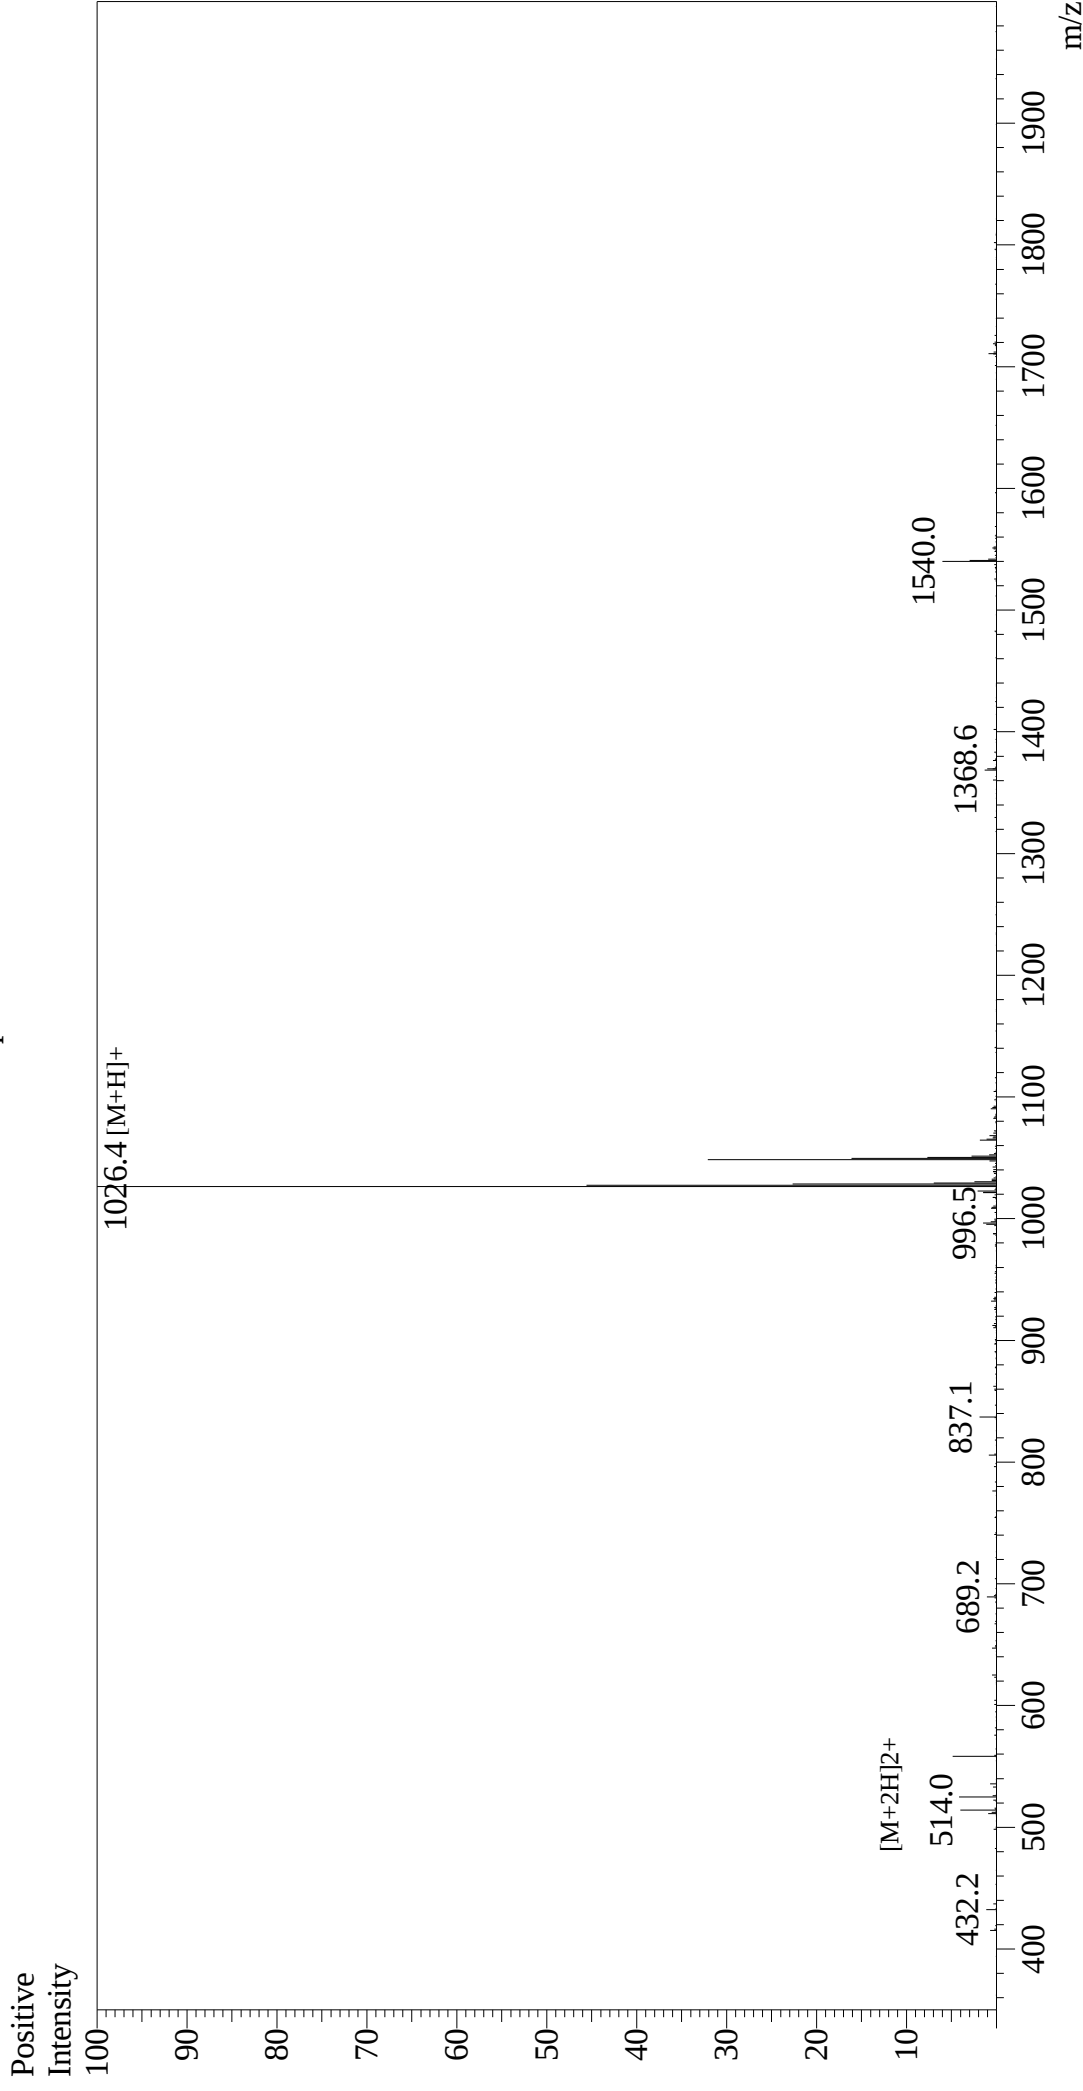

Sample Information		Equipment : ZJ21010035	
Month-Day Processed :	02/05/24	Interface Bias : +4.5 kV	
Time Processed :	16:01:09	Drying Gas Flow : 5 L/min	
Injection Volume :	0.3	T.Flow : 0.2 ml/min	
Sample Name :	Influenza A NP(366-374) Strain A/PR/8/35	B.conc : 50%H2O/50%MeOH	
Cat No. :	RP20267		
Lot No. :	E4429724A		
Theoretical MW :	1026.12		
Observed MW :	1025.4		