

Sample Name :Substance P
Cat No. :RP10178
Lot No. :E4710723A
Time Processed :5:20:17
Month-Day-Year Processed :01/29/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ19010141

<Chromatogram>

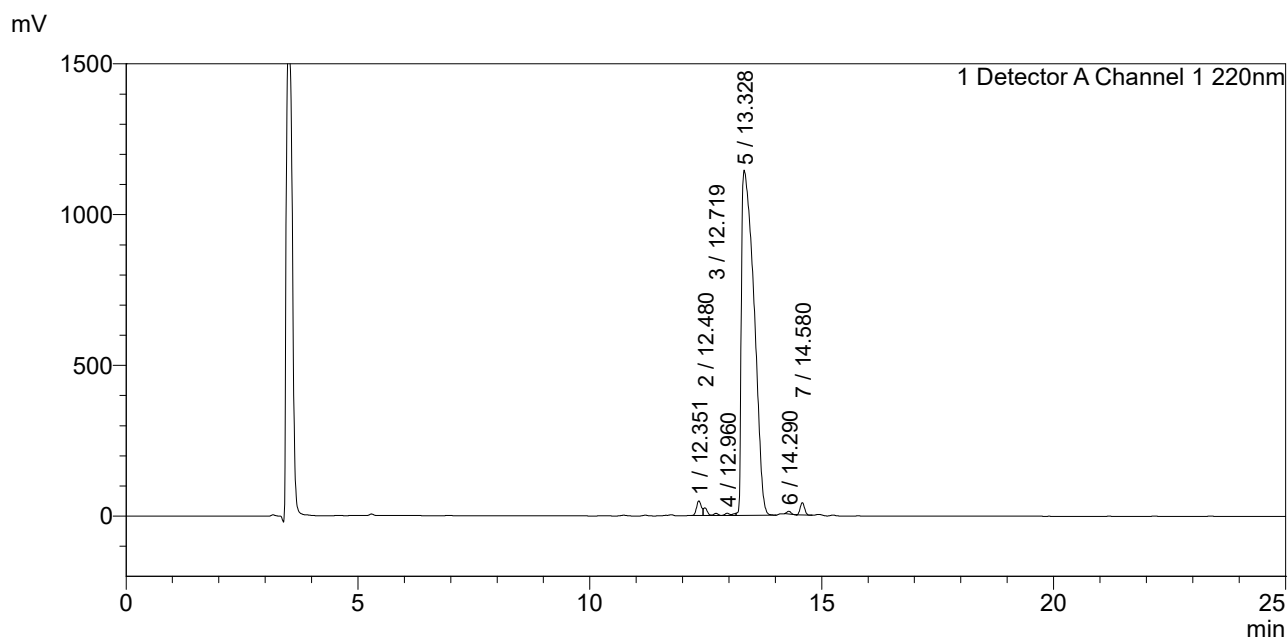

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.351	355756	48624	1.582
2	12.480	139025	25053	0.618
3	12.719	43854	6965	0.195
4	12.960	78836	7264	0.351
5	13.328	21542875	1145097	95.822
6	14.290	55851	9223	0.248
7	14.580	266031	41011	1.183
Total		22482228	1283238	100.000