


Mass Spectrum

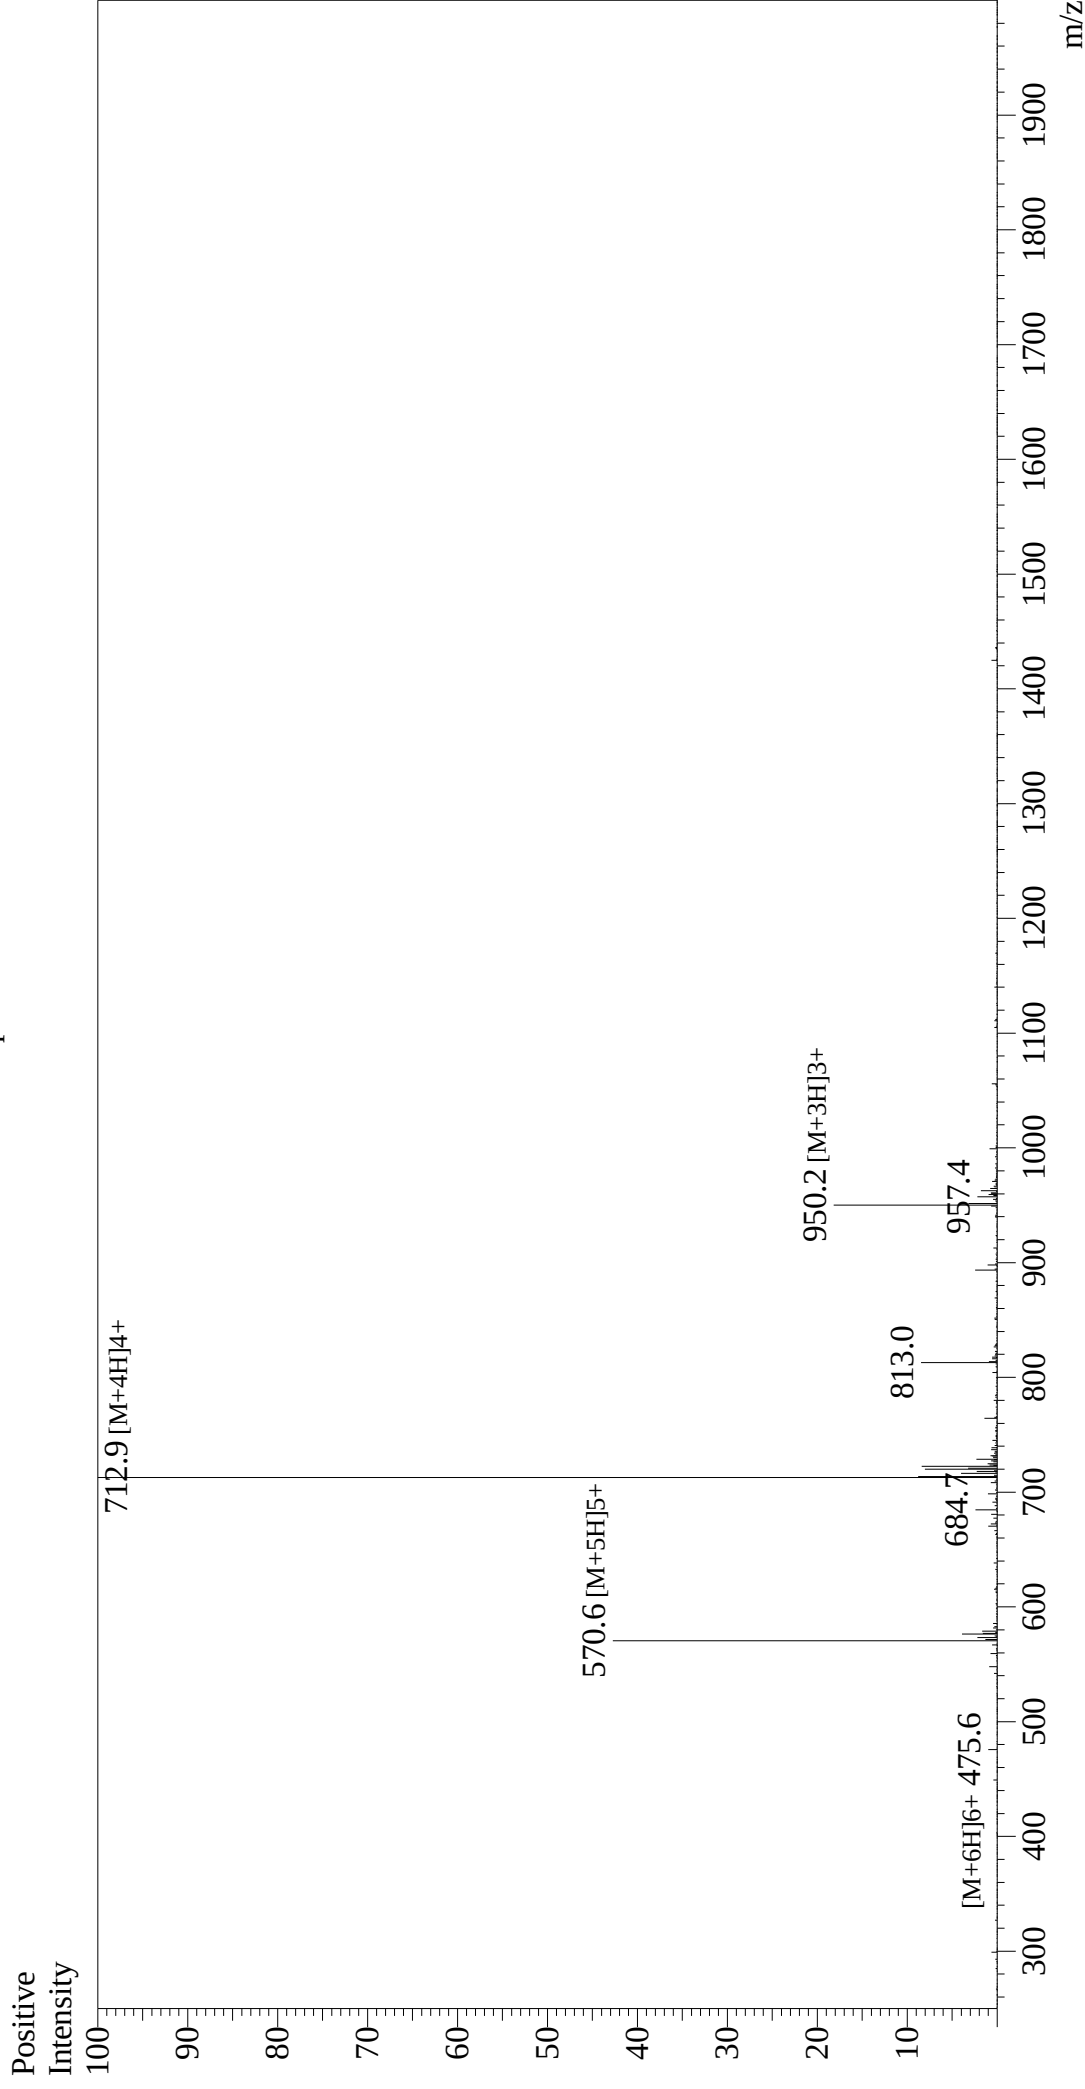

Sample Information

Month-Day Processed : 06/16/23
 Time Processed : 3:51:07 PM
 Injection Volume : 0.3
 Sample Name : Melittin, honey bee
 Cat No. : RP20415
 Lot No. : E472223F
 Theoretical MW : 2847.50
 Observed MW : 2847.6

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : ZJ22010150
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH