

Sample Name :Glucagon-Like Peptide (GLP) II, human

Cat No. :RP10769

Lot No. :E4773126E

Time Processed :15:48:52

Month-Day-Year Processed :04/25/2026

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ25010053

<Chromatogram>

mV

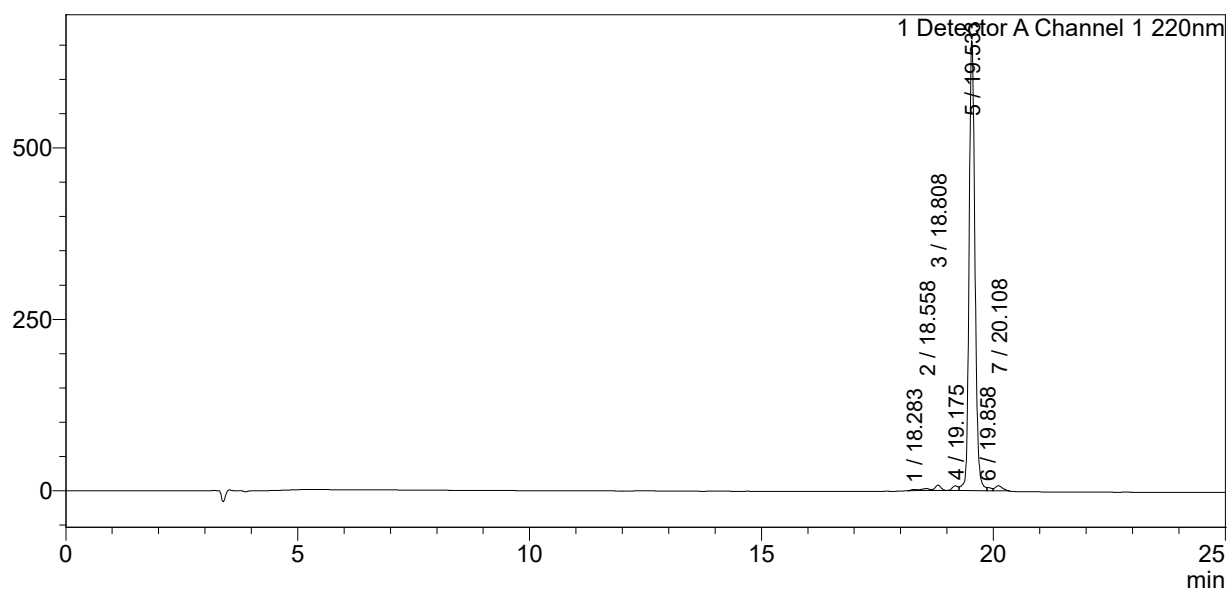

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	18.283	15365	1779	0.254
2	18.558	35088	2948	0.580
3	18.808	68680	7858	1.136
4	19.175	60056	6901	0.993
5	19.533	5751614	656426	95.103
6	19.858	32803	4760	0.542
7	20.108	84190	7590	1.392
Total		6047795	688262	100.000