

Sample Name :Substance P
Cat No. : RP10178
Lot No. : E4863724I
Time Processed :19:44:55
Month-Dav-Year Processed :09/21/2024
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ17010508

<Chromatogram>

mV

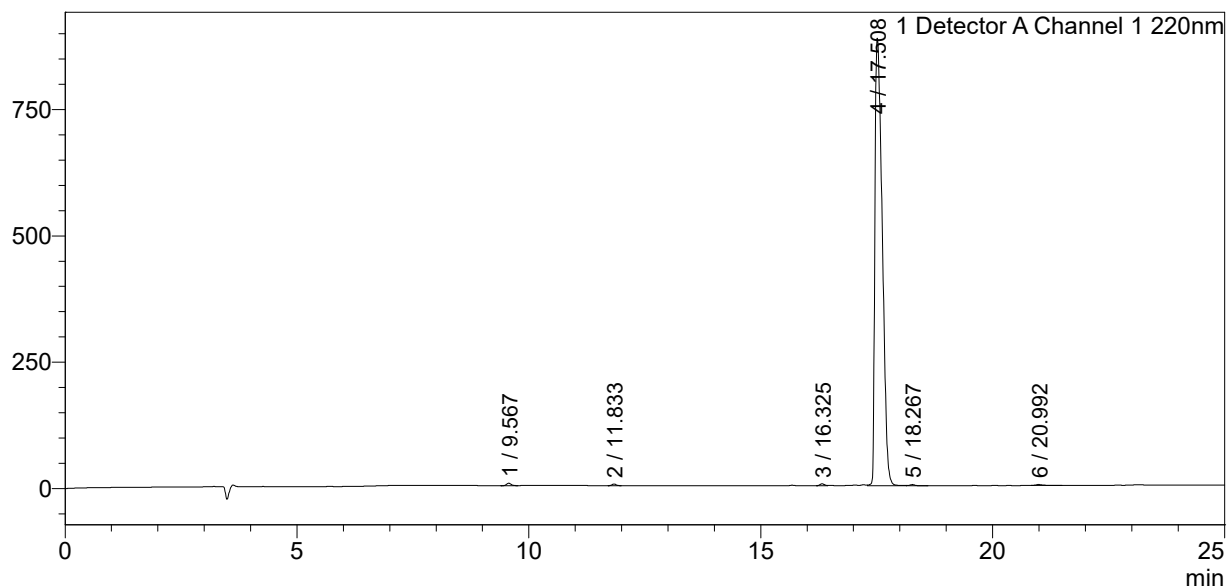

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.567	33888	4915	0.345
2	11.833	18603	3218	0.189
3	16.325	24973	3773	0.254
4	17.508	9709597	885846	98.845
5	18.267	16633	2207	0.169
6	20.992	19327	1786	0.197
Total		9823021	901744	100.000