


Mass Spectrum

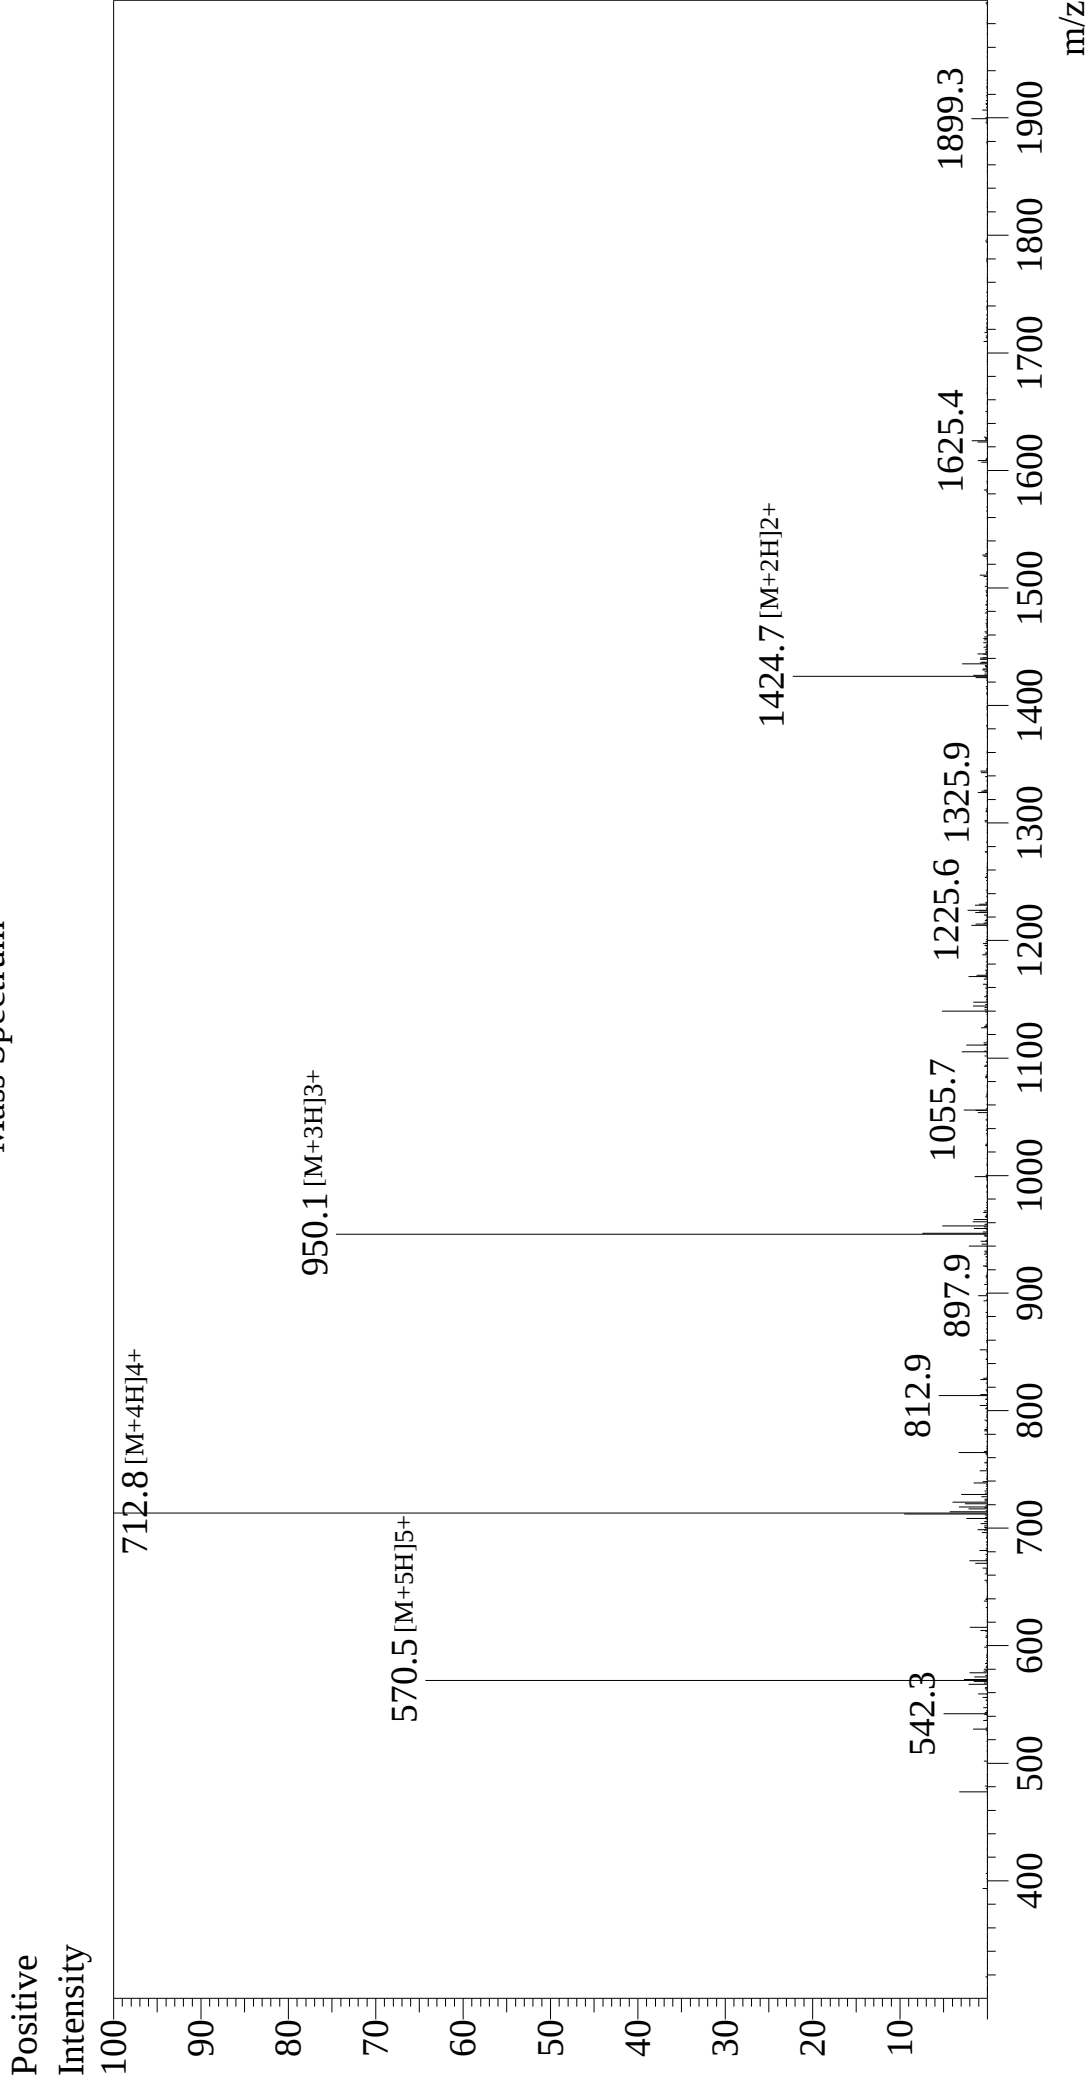

Sample Information

Month-Day Processed : 09/21/24
Time Processed : 13:17:29
Injection Volume : 0.2
Sample Name : Melittin, honey bee
Cat No. : RP20415
Lot No. : E4871024I
Theoretical MW: 2847.50
Observed MW : 2847.2

Interface

Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment

Interface Bias
Drying Gas Flow
T.Flow
B.conc

:ZJ22010150
: +4.5 kV
:5 L/min
:0.2 ml/min
:50%H2O/50%M