


Mass Spectrum

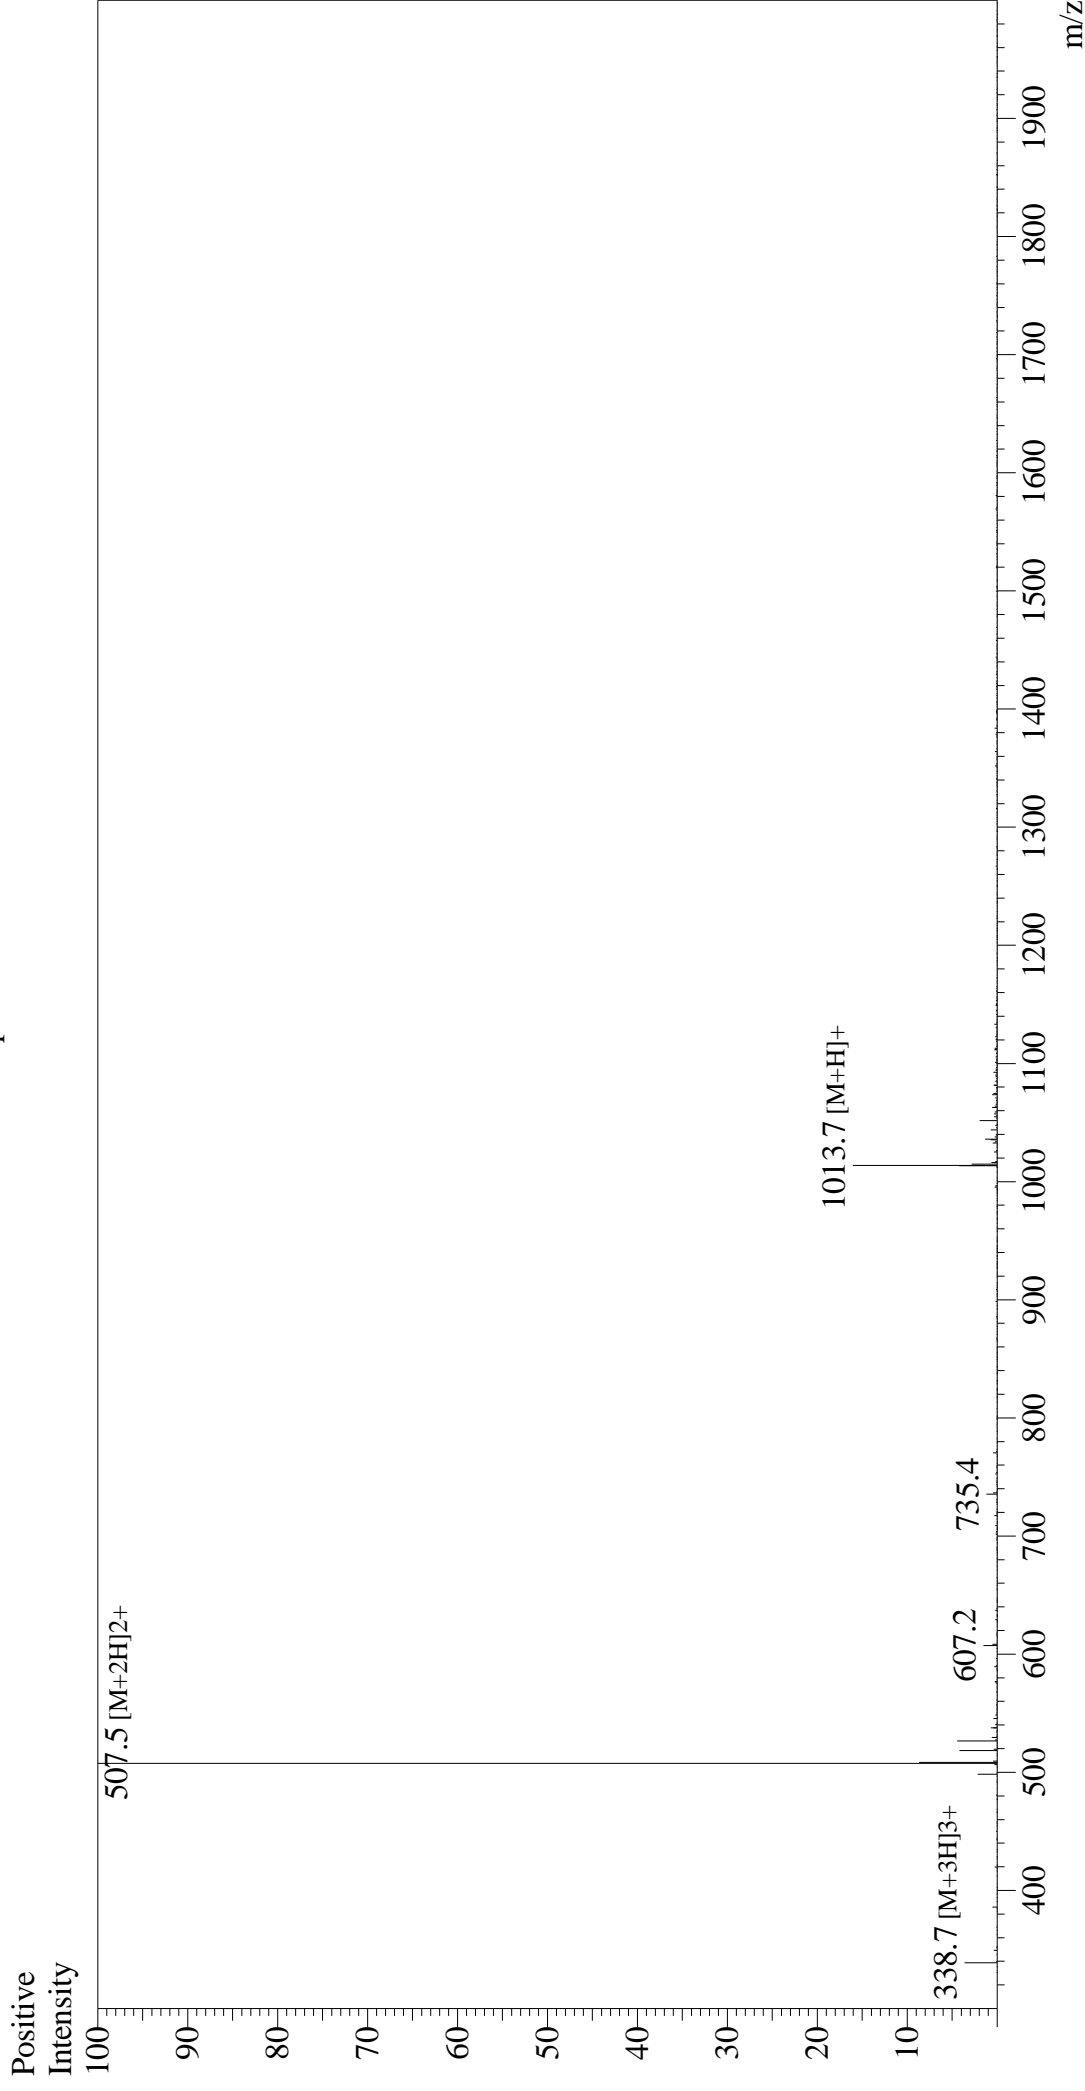

Sample Information

Month-Day Processed :	10/24/22	Equipment	:ZJ22010150
Time Processed :	3:23:49 PM	Interface Bias	: +4.5 kV
Injection Volume :	0.1	Drying Gas Flow	:5 L/min
Sample Name :	DYKDDDDK Peptide	T.Flow	:0.2 ml/min
Cat No. :	RP10586	B.conc	:50%H2O/50%MeOH
Lot No. :	E4981122J		
Theoretical MW:1012.97			
Observed MW :1013.0			