

Sample Name :Substance P
Cat No. : RP10178
Lot No. : E5052925C
Time Processed :12:57:16
Month-Day-Year Processed :03/07/2025

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ21010026

<Chromatogram>

mV

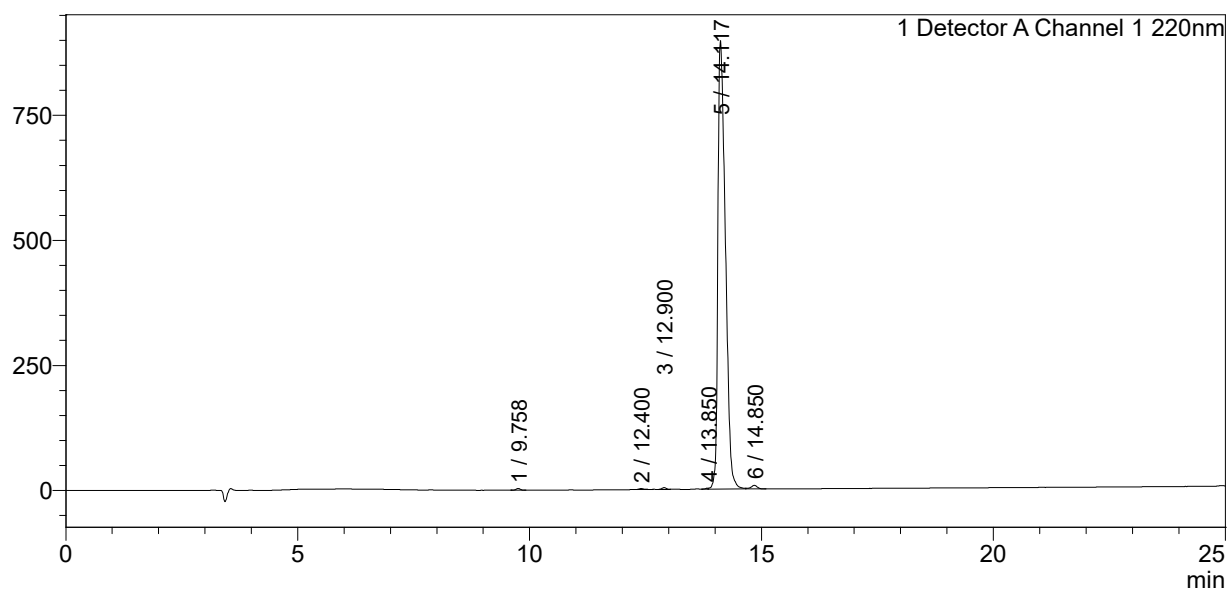

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.758	21913	3593	0.214
2	12.400	16642	2028	0.163
3	12.900	23147	3477	0.226
4	13.850	8243	1947	0.081
5	14.117	10095422	896667	98.639
6	14.850	69364	7221	0.678
Total		10234731	914932	100.000