


Mass Spectrum

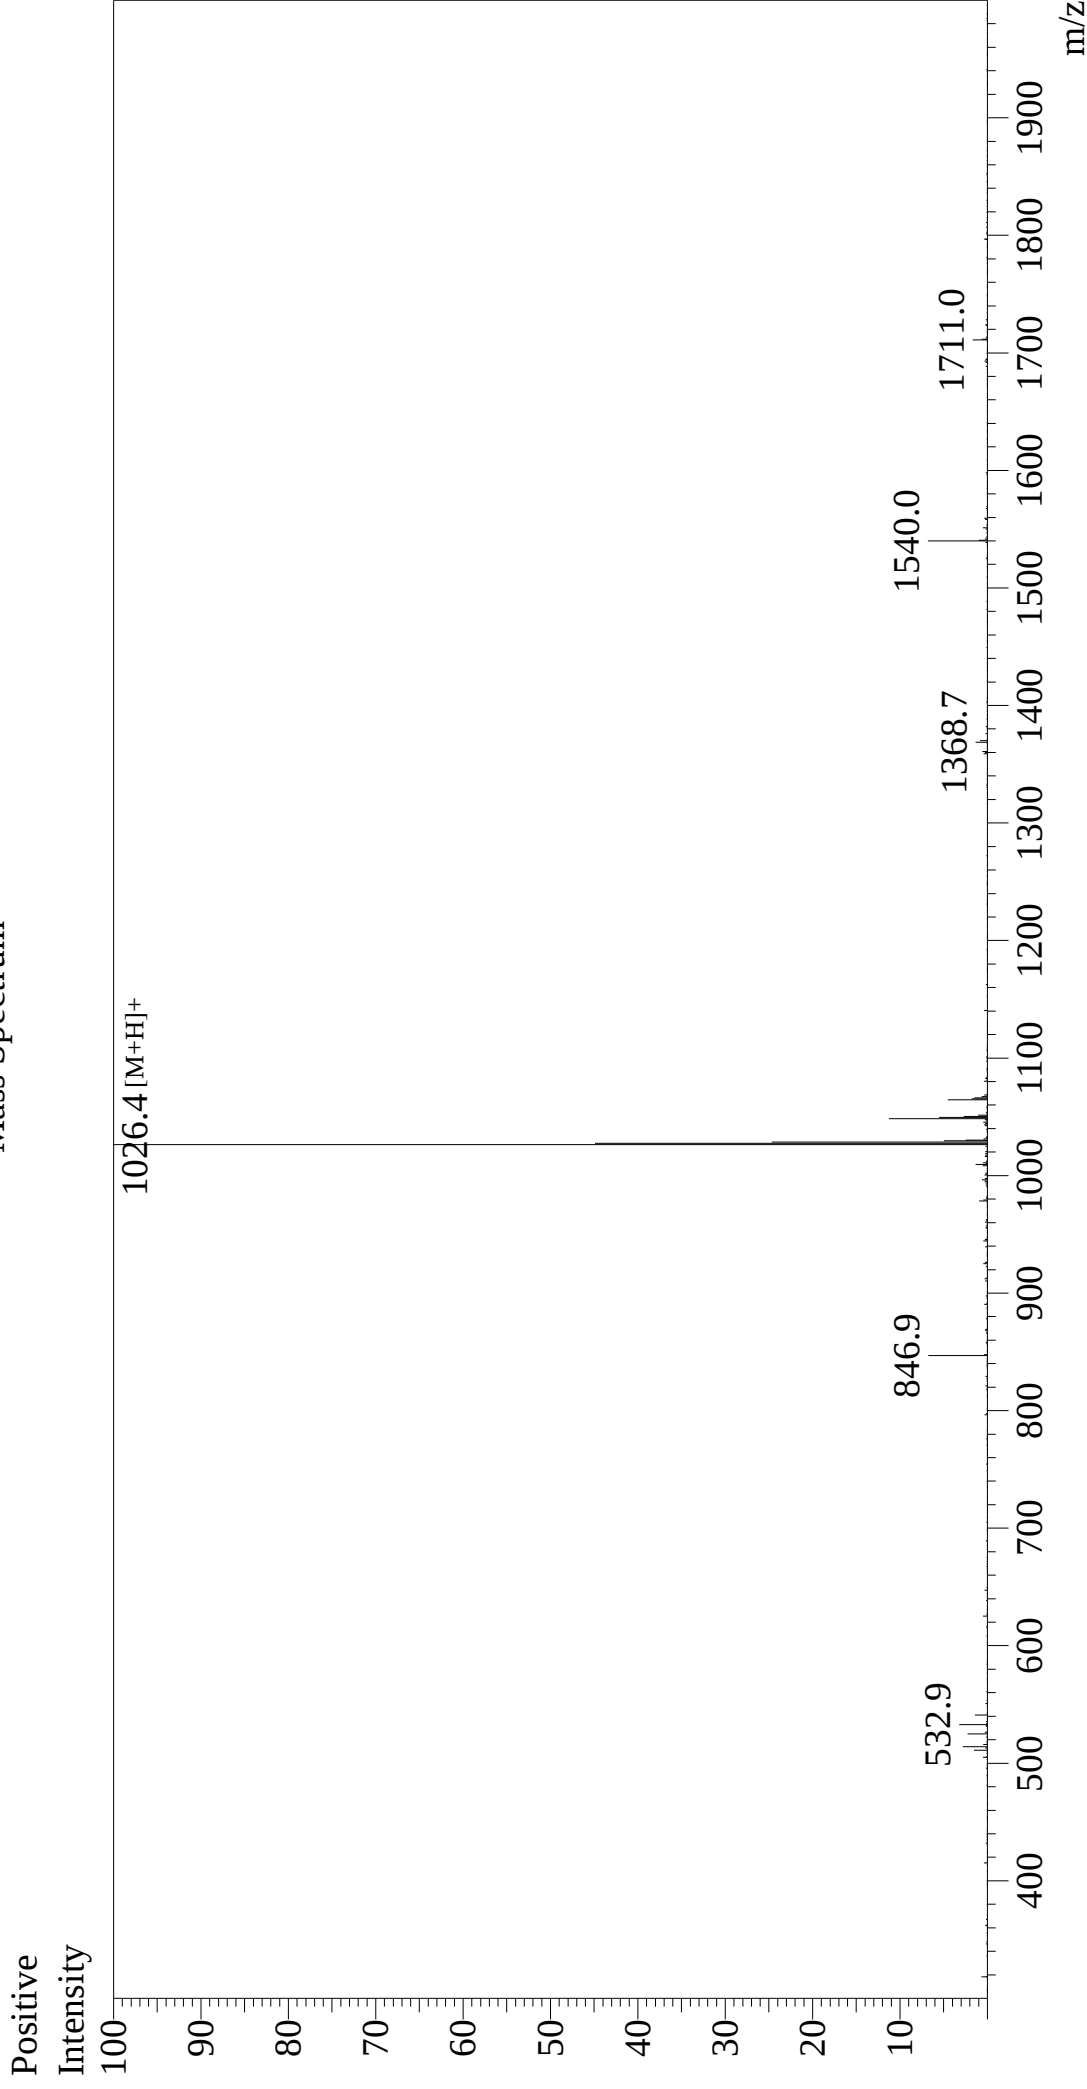

Sample Information		Interface	:ESI	Equipment	:ZJ22010150
Month-Day Processed :	05/15/24	Nebulizing Gas Flow	:1.5L/min	Interface Bias	: +4.5 kV
Time Processed :	15:05:29	CDL Temp	:250	Drying Gas Flow	:5 L/min
Injection Volume :	0.2	Block Temp	:200	T.Flow	:0.2 ml/min
Sample Name :	Influenza A NP(366-374) Strain A/PR/8/35			B.conc	:50%H ₂ O/50%MeOH
Cat No. :	RP20267				
Lot No. :	E5089524E				
Theoretical MW:	1026.12				
Observed MW :	1025.4				