
Mass Spectrum

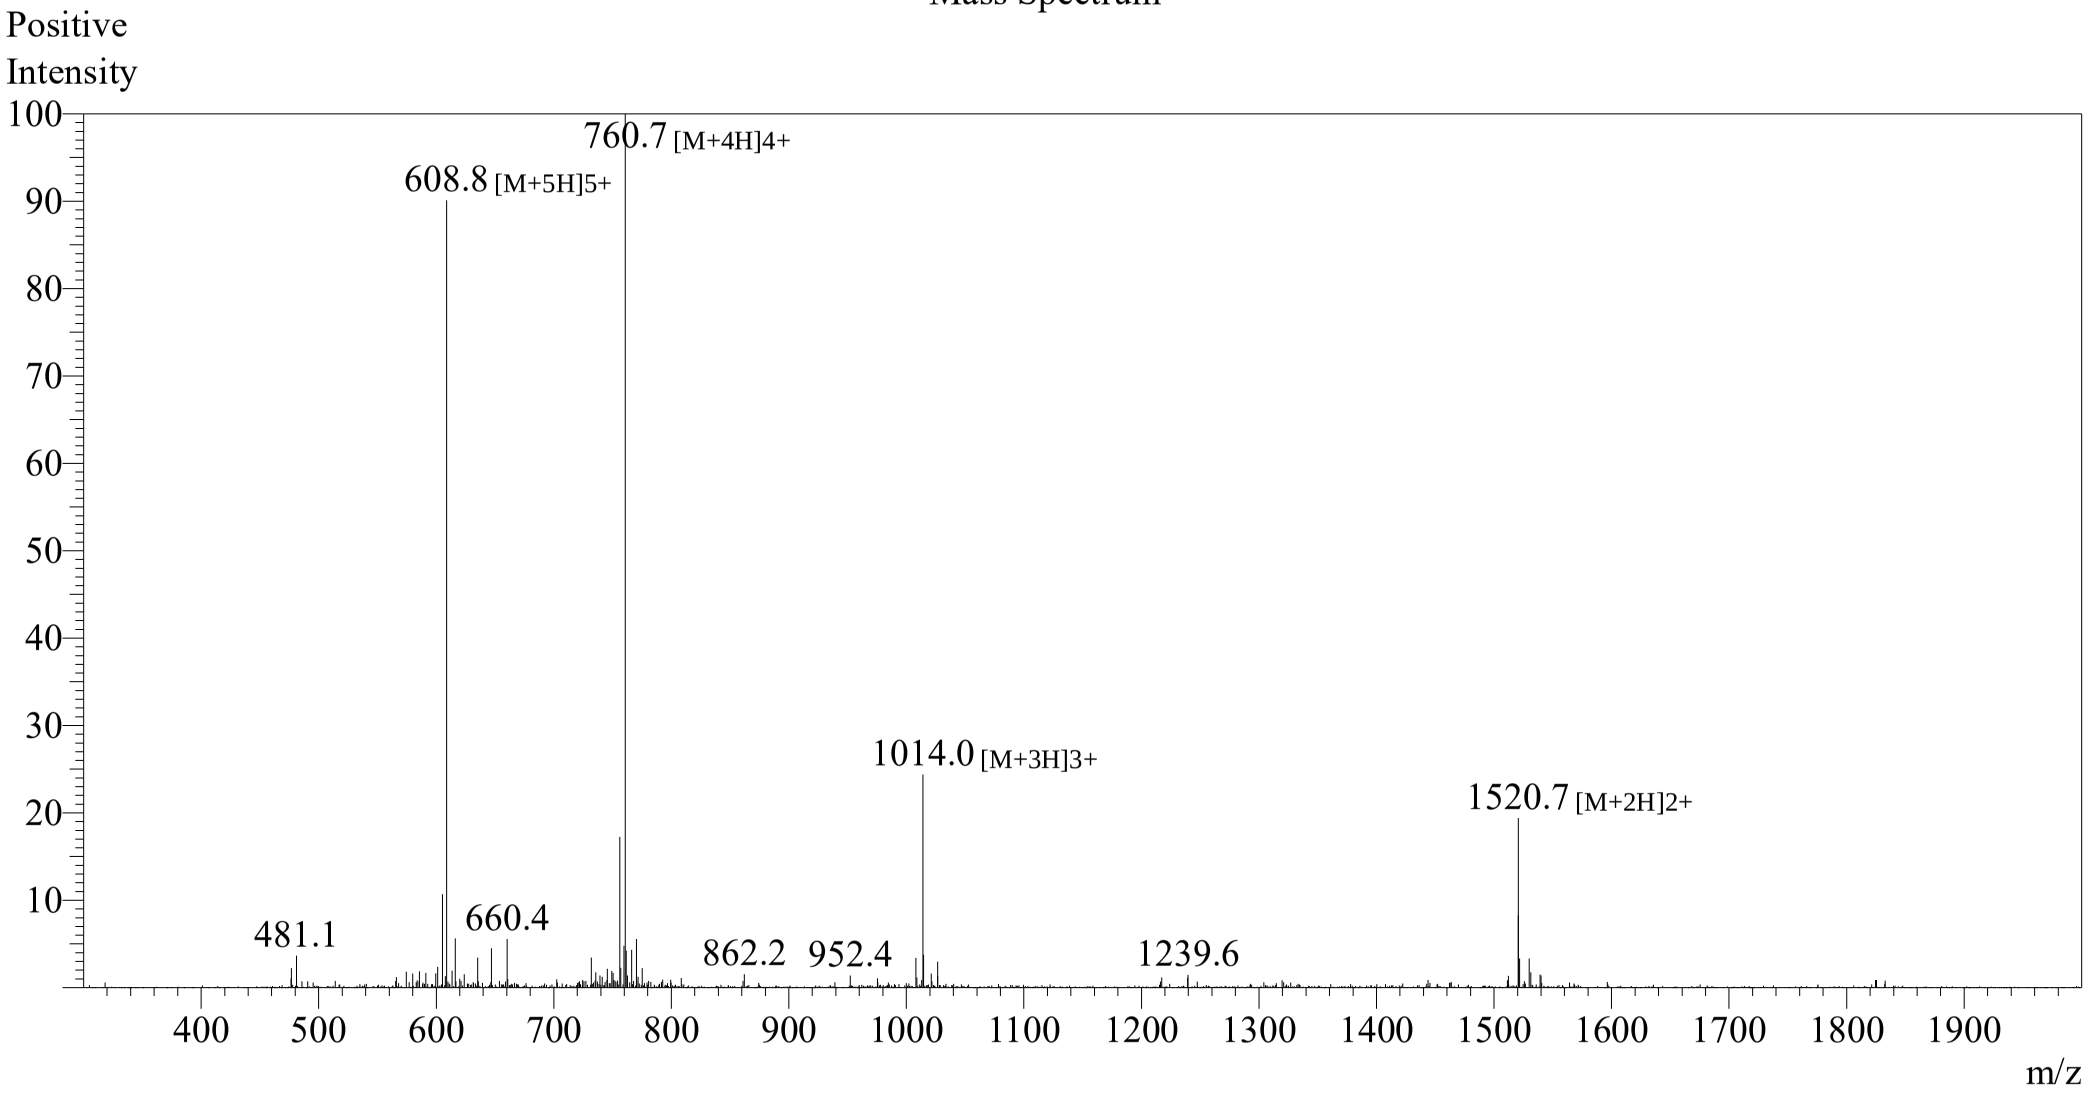

Sample Information
Month-Day Processed : 06/30/26
Time Processed : 8:51:04
Injection Volume : 0.5
Sample Name : Secretin, human
Cat No. : RP10249
Lot No. : E5103926F
Theoretical MW:3039.50
Observed MW : 3038.8

Interface :ESI
Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H2O/50%MeOH