


# Mass Spectrum

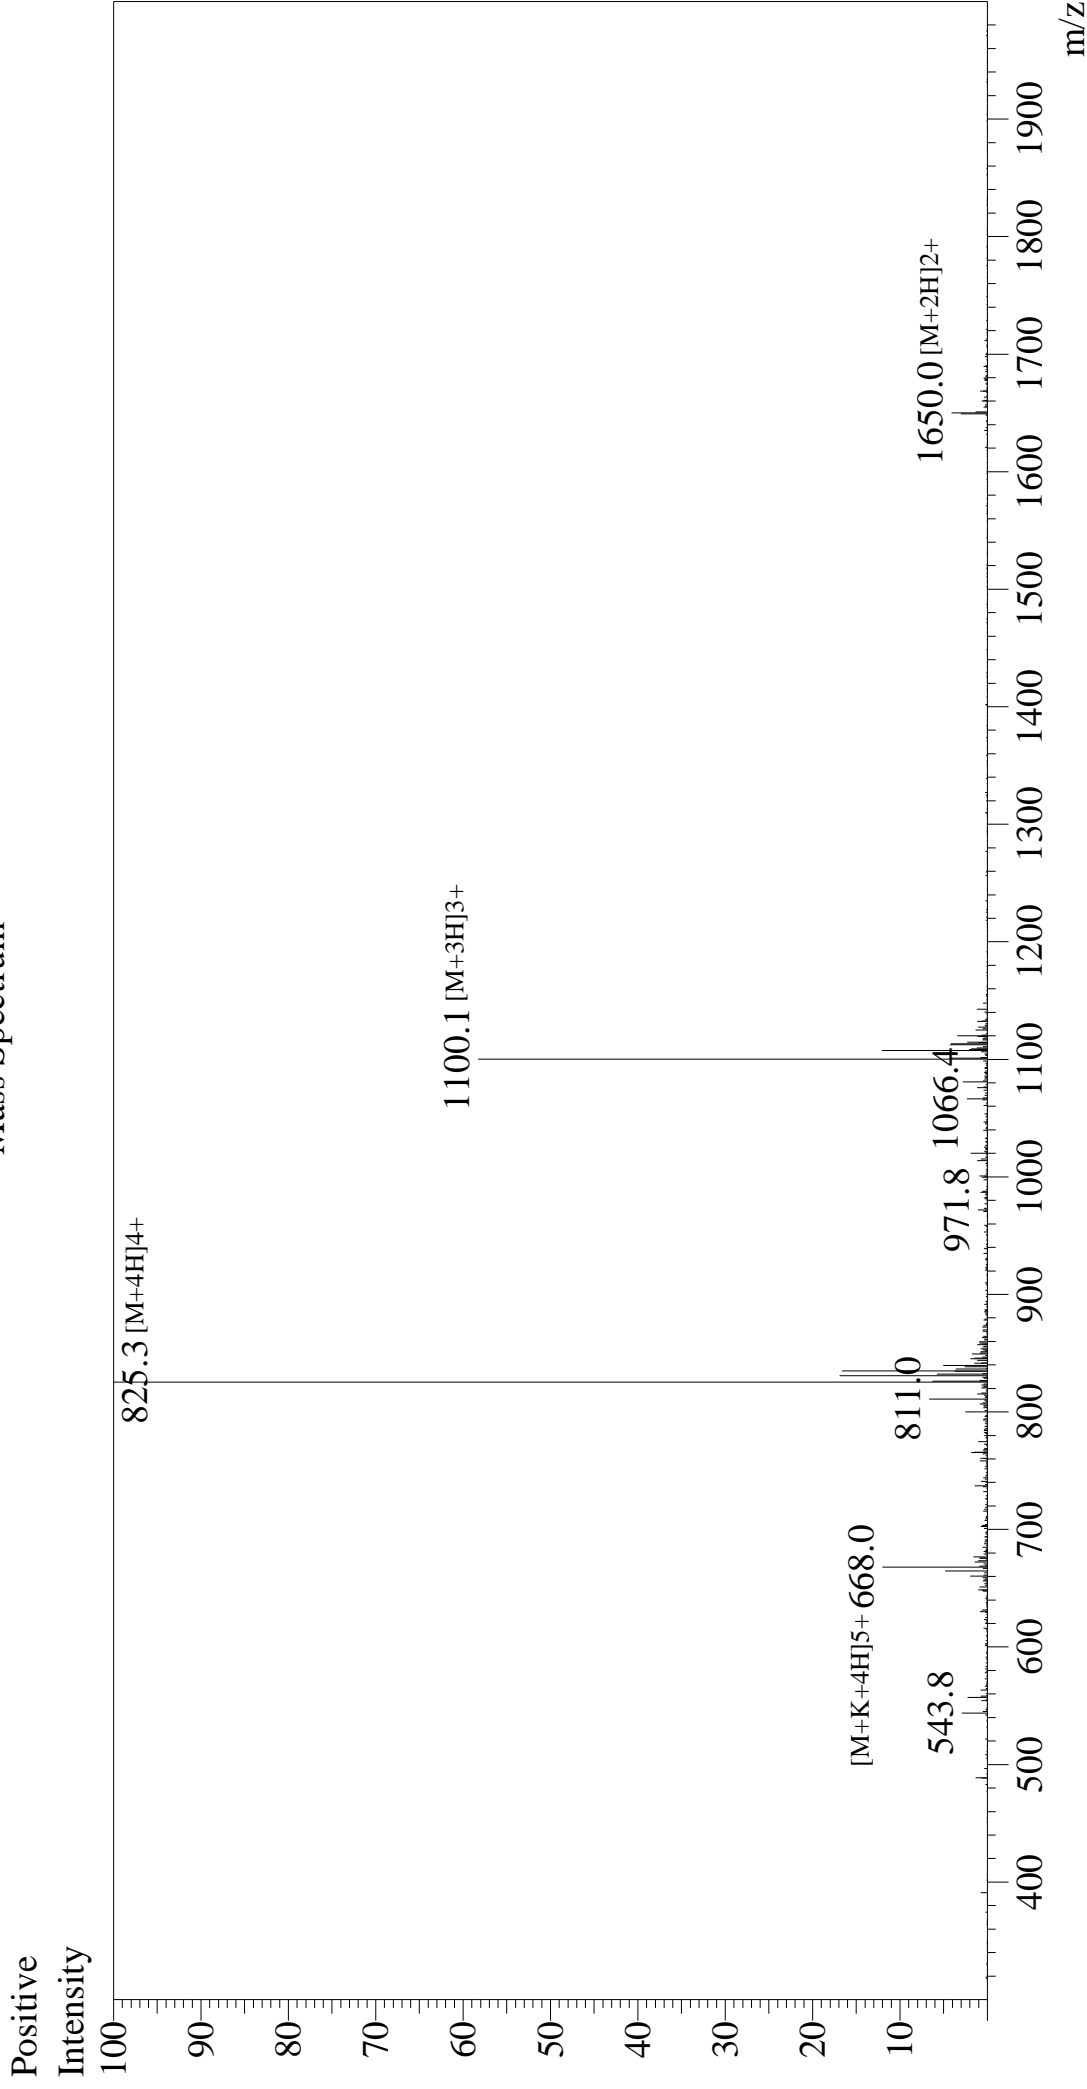

## Sample Information

|                          |                                                    |                     |           |                 |              |
|--------------------------|----------------------------------------------------|---------------------|-----------|-----------------|--------------|
| Month-Day Processed :    | 01/27/23                                           | Interface           | :ESI      | Equipment       | : ZI21010035 |
| Time Processed :         | 18:49:42                                           | Nebulizing Gas Flow | :1.5L/min | Interface Bias  | : +4.5 kV    |
| Injection Volume :       | 0.2                                                | CDL Temp            | :250      | Drying Gas Flow | :5 L/min     |
| Sample Name :            | Glucagon-Like Peptide (GLP) I (7-36), amide, human | Block Temp          | :200      | T.Flow          | :0.2 ml/min  |
| Cat No. :                | RP10773                                            |                     |           | B.conc          | :50%H2O/50%M |
| Lot No. :                | E5293323A                                          |                     |           |                 |              |
| Theoretical MW : 3297.50 |                                                    |                     |           |                 |              |
| Observed MW : 3297.2     |                                                    |                     |           |                 |              |