

Sample Name :Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E5313524K
Time Processed :0:38:51
Month-Day-Year Processed :11/22/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
Equipment: ZJ19010141

<Chromatogram>

mV

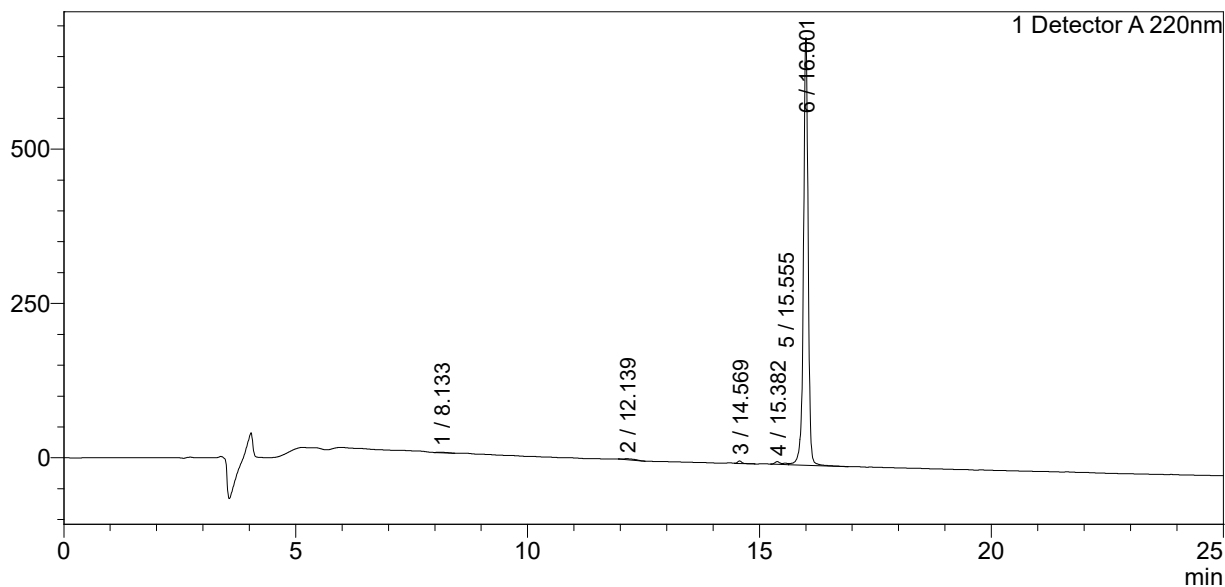

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.133	8660	609	0.173
2	12.139	30735	1558	0.615
3	14.569	27986	4311	0.560
4	15.382	32765	4463	0.656
5	15.555	17944	2211	0.359
6	16.001	4875883	692832	97.635
Total		4993973	705983	100.000