

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E5317624K
Time Processed :14:45:25
Month-Day-Year Processed :11/26/2024
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 5 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 27.00 | Pumps | B.Conc | 95 |
| 27.01 | Pumps | B.Conc | 5 |
| 35.00 | Pumps | B.Conc | 5 |
| 35.01 | Controller | Stop | |

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ19010325

<Chromatogram>

mV

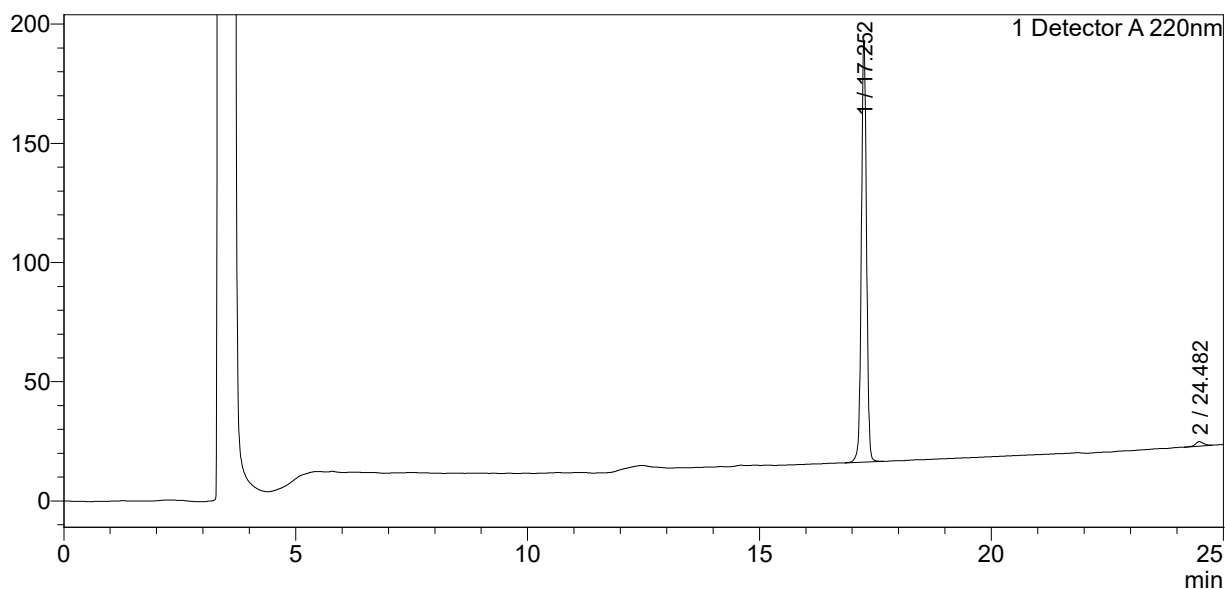

<Peak Table>

Detector A 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 17.252 | 1356784 | 176801 | 98.378 |
| 2 | 24.482 | 22364 | 1887 | 1.622 |
| Total | | 1379148 | 178688 | 100.000 |