

Sample Name :Substance P  
 Cat No. : RP10178  
 Lot No. : E5341722K  
 Time Processed :18:11:57  
 Month-Day-Year Processed :11/25/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: SS-CM-0286

### <Chromatogram>

mV

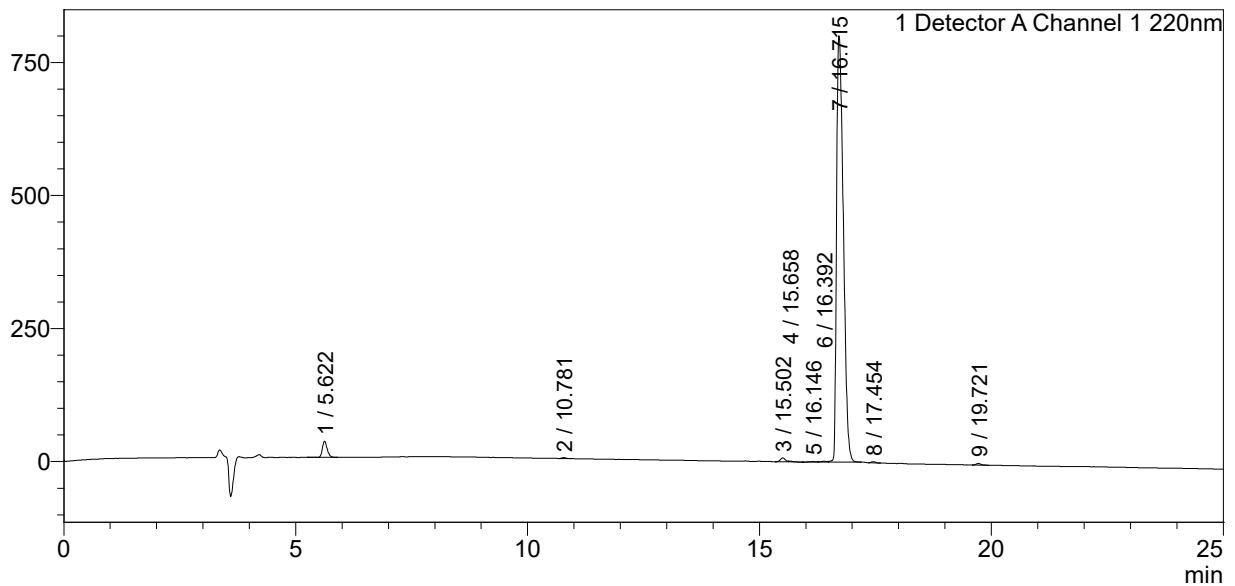

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.622	219124	30399	2.582
2	10.781	10578	1696	0.125
3	15.502	55444	7368	0.653
4	15.658	10250	1620	0.121
5	16.146	11552	979	0.136
6	16.392	15711	1658	0.185
7	16.715	8127263	801618	95.778
8	17.454	13747	2180	0.162
9	19.721	21857	3020	0.258
Total		8485526	850539	100.000