

Sample Name :IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E5402122J
 Time Processed :8:39:11
 Month-Day-Year Processed :11/02/2022

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
10.00	Pumps	B.Conc	35
35.00	Pumps	B.Conc	95
37.00	Pumps	B.Conc	95
37.01	Pumps	B.Conc	5
45.00	Pumps	B.Conc	5
45.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

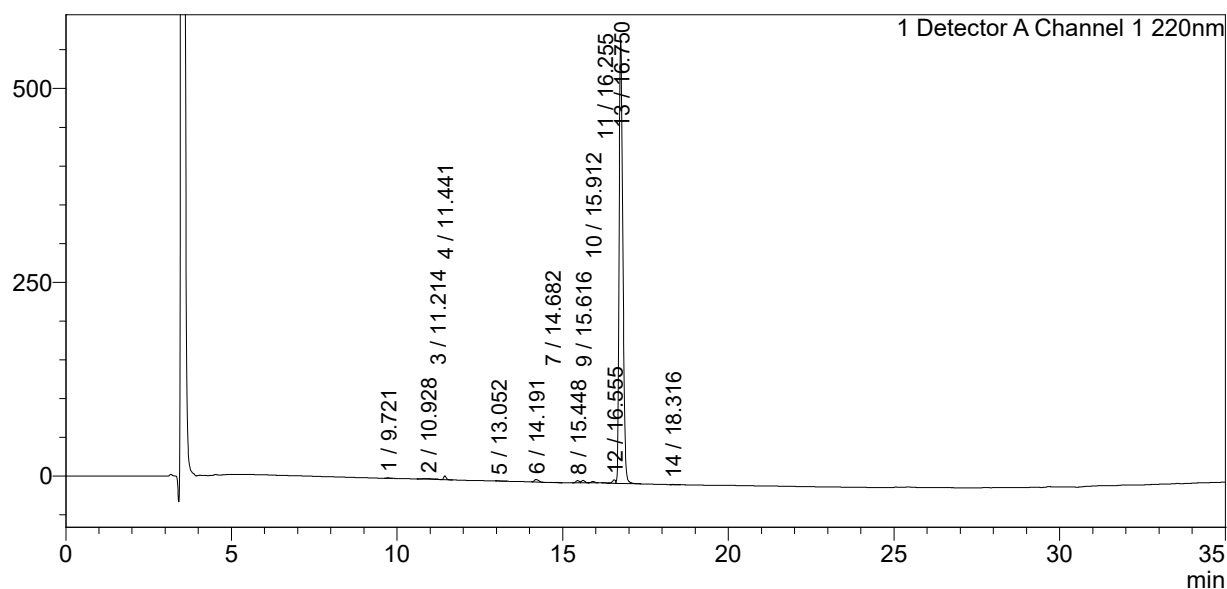

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.721	3700	717	0.080
2	10.928	11523	676	0.249
3	11.214	1967	479	0.043
4	11.441	26279	5011	0.568
5	13.052	1466	157	0.032
6	14.191	28879	3315	0.624
7	14.682	1278	90	0.028
8	15.448	21130	3024	0.457
9	15.616	22846	3248	0.494
10	15.912	14184	1871	0.306
11	16.255	1723	323	0.037
12	16.555	28685	4333	0.620
13	16.750	4462944	571273	96.437
14	18.316	1248	159	0.027
Total		4627851	594676	100.000