

Sample Name : HA Peptide
 Cat No. : RP11735
 Lot No. : E5409723L
 Time Processed : 9:47:37
 Month-Day-Year Processed : 12/31/2023
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm

Equipment: GK11010009

<Chromatogram>

mV

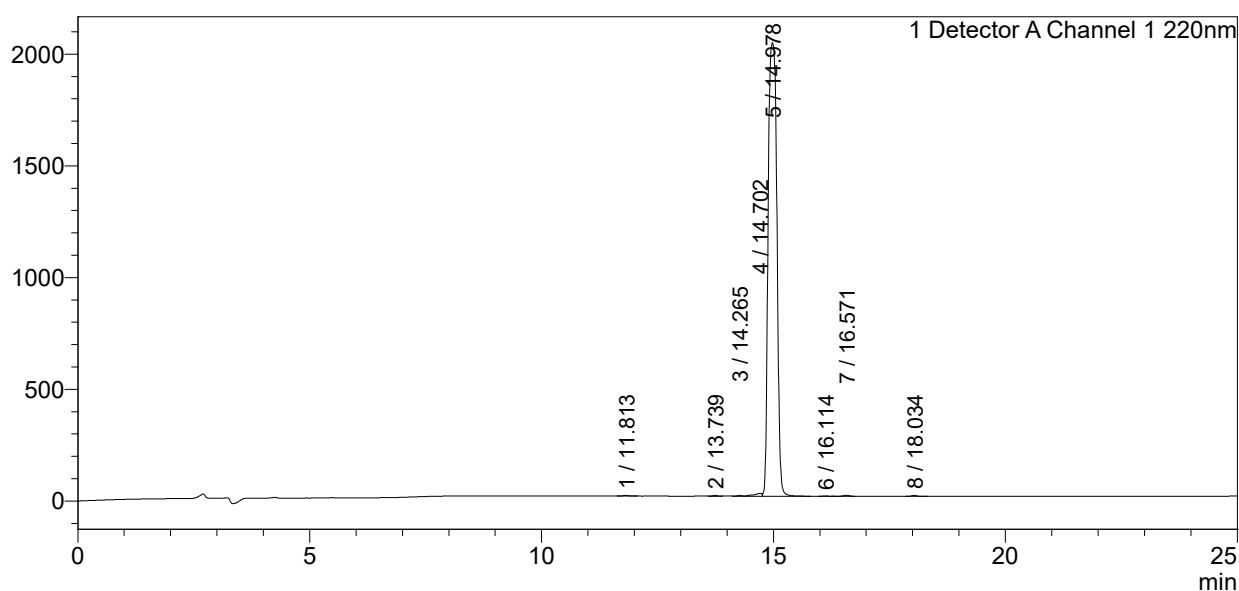

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.813	24669	3140	0.093
2	13.739	31007	3569	0.117
3	14.265	28176	3491	0.106
4	14.702	159332	12775	0.599
5	14.978	26259244	2030248	98.750
6	16.114	13052	1887	0.049
7	16.571	42812	4416	0.161
8	18.034	33446	4048	0.126
Total		26591736	2063574	100.000