


Mass Spectrum

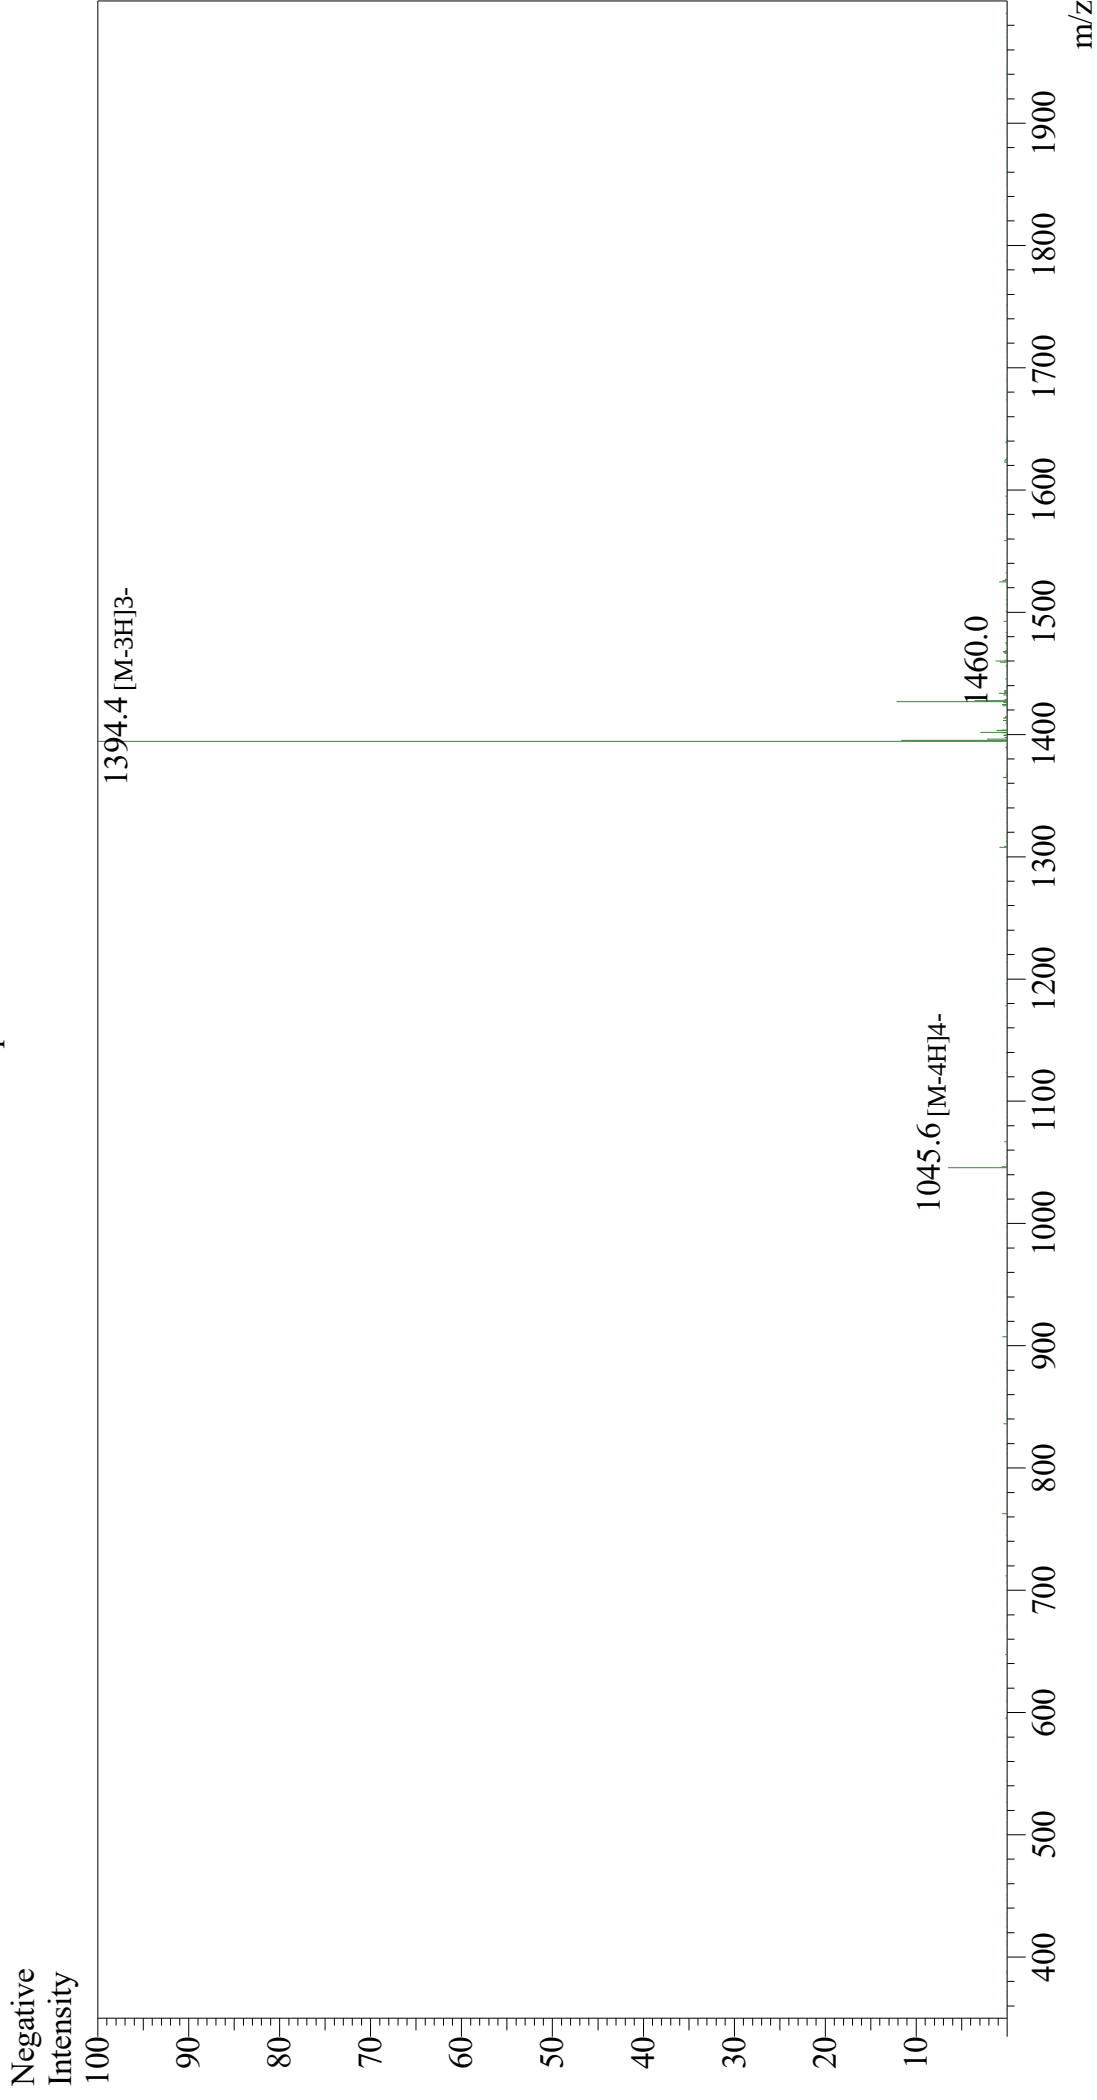

Sample Information
Month-Day Processed : 08/04/26
Time Processed : 18:05:51
Injection Volume : 0.3
Sample Name : Exendin-4
Cat No. : RP10874
Lot No. : E5425126H
Theoretical MW : 4186.66
Observed MW : 4186.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200
Equipment : ZJ21010035
Interface Bias : -3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH