

Sample Name :IRBP (1-20), human
Cat No. : RP20269
Lot No. : E5534023B
Time Processed :8:44:37 AM
Month-Day-Year Processed :03/07/2023
Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
Equipment: ZJ17010508

<Chromatogram>

mV

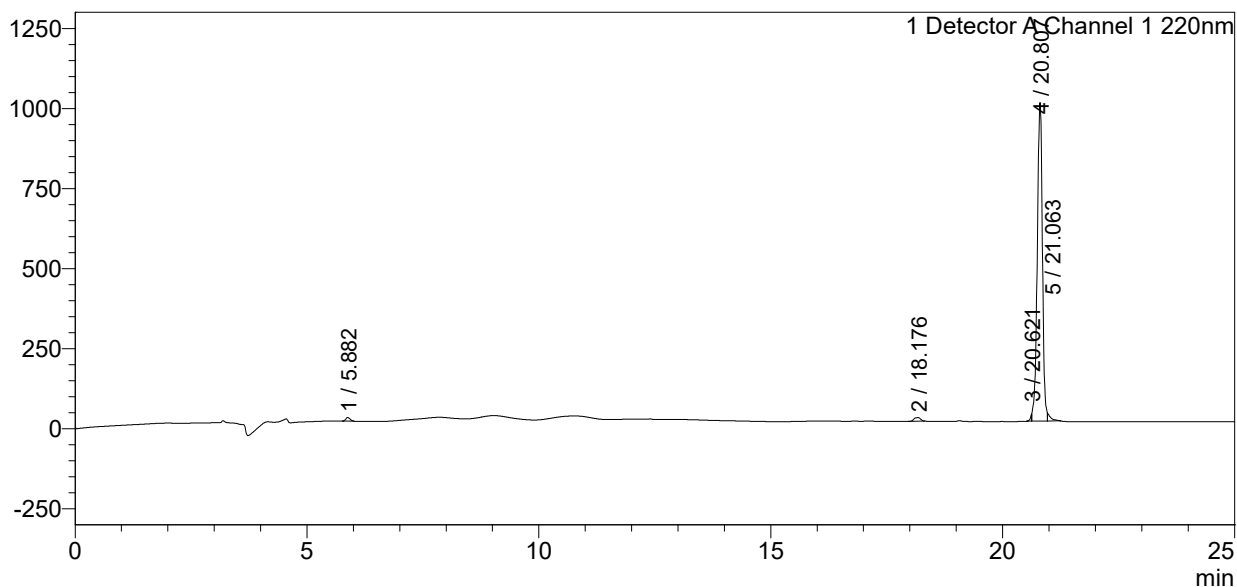

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.882	70882	11414	0.879
2	18.176	106153	10978	1.316
3	20.621	43665	17807	0.542
4	20.807	7732029	994478	95.890
5	21.063	110703	7575	1.373
Total		8063432	1042252	100.000