


Mass Spectrum

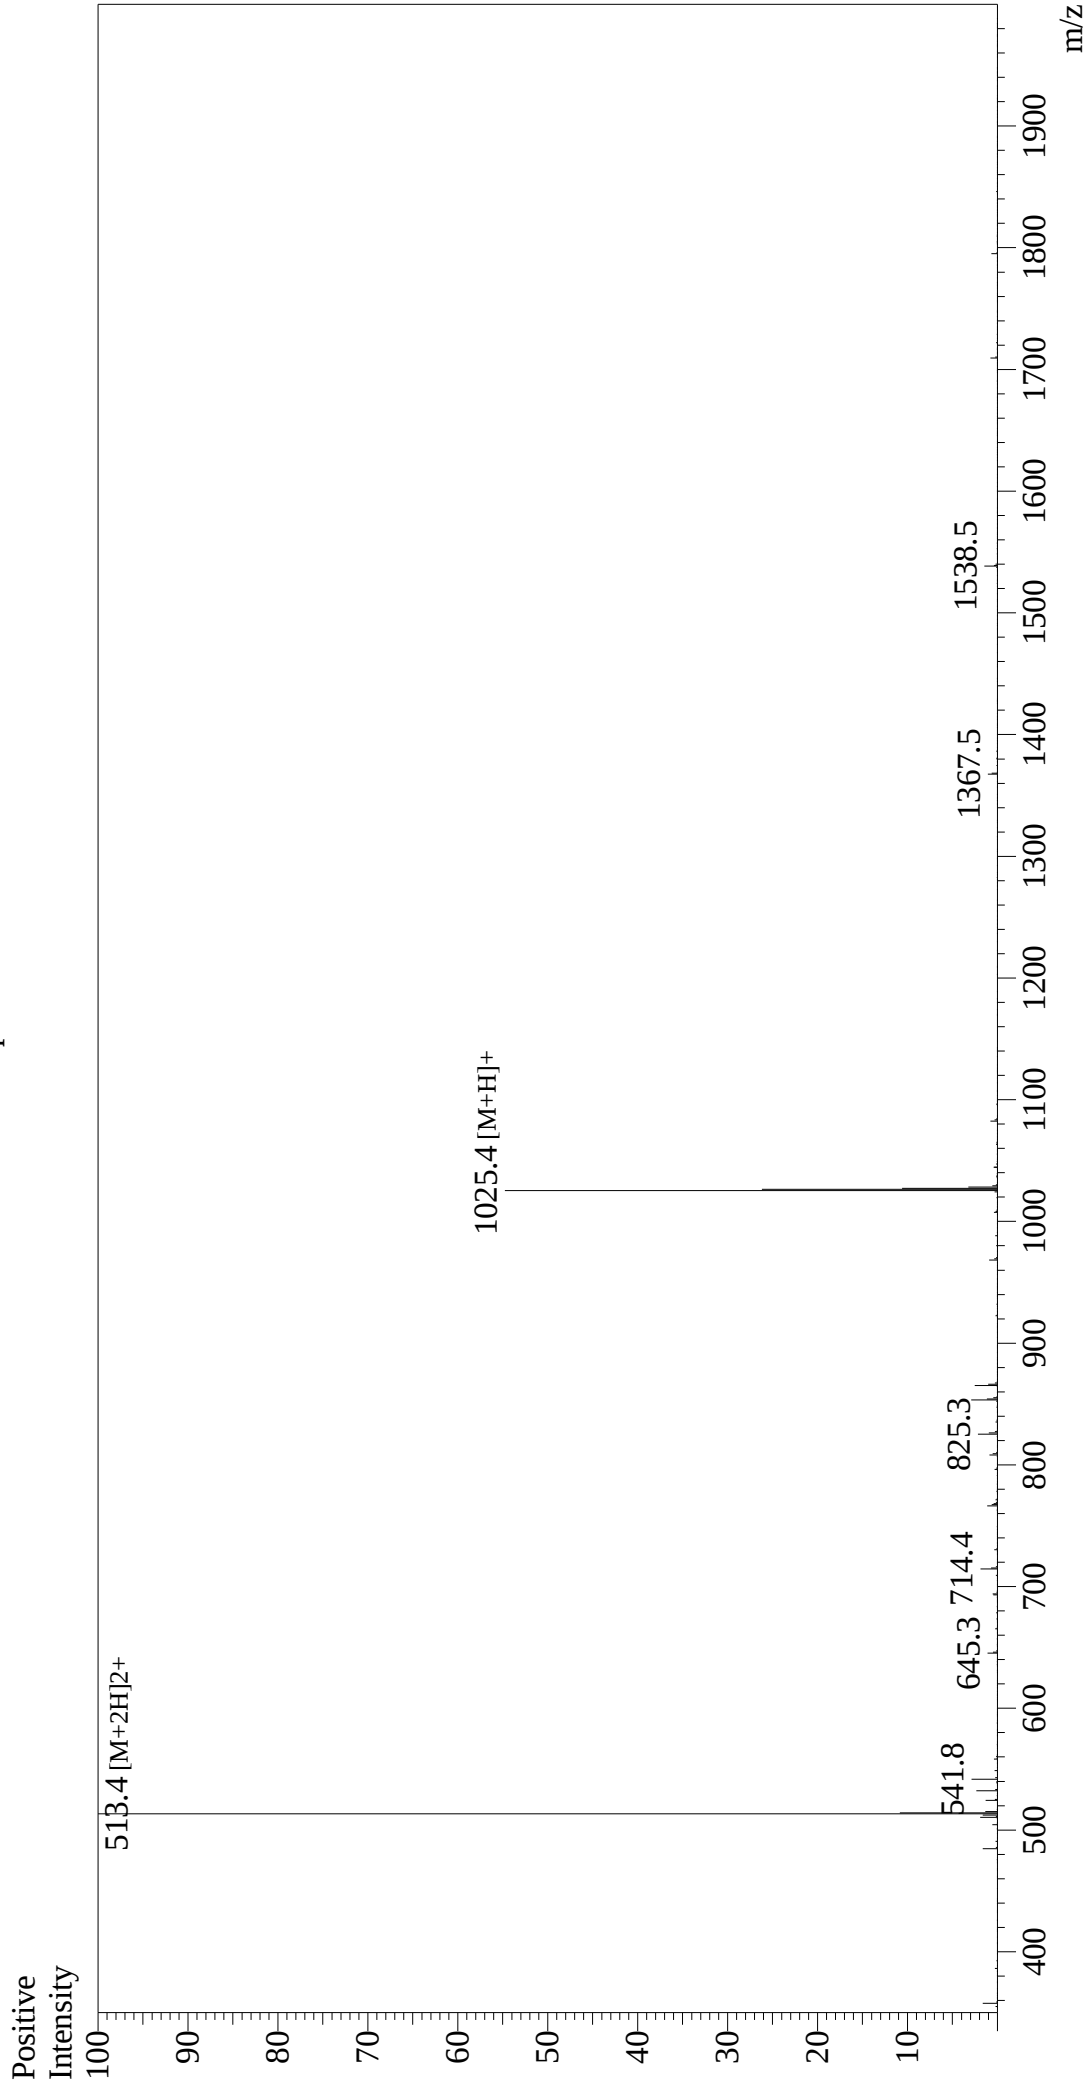

Sample Information

Month-Day Processed : 07/24/25

Time Processed : 22:44:04

Injection Volume : 0.2

Sample Name : RGD

Cat No. : RP20297

Lot No. : E5787825G

Theoretical MW: 1025.06

Observed MW : 1024.8

Interface

Nebulizing Gas Flow :1.5L/min

CDL Temp :250

Block Temp :200

:ESI

:ESI

:250

:200

Equipment

: ZJ21010035

Interface Bias : +4.5 kV

Drying Gas Flow :5 L/min

T.Flow :0.2 ml/min

B.conc :50%H₂O/50%MeOH