

Sample Name :KRAS G12V Peptide (VVVGAVGVGK)

Cat No. : RP30229

Lot No. : E5801123K

Time Processed :20:00:20

Month-Day-Year Processed :11/12/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ20010139

<Chromatogram>

mV

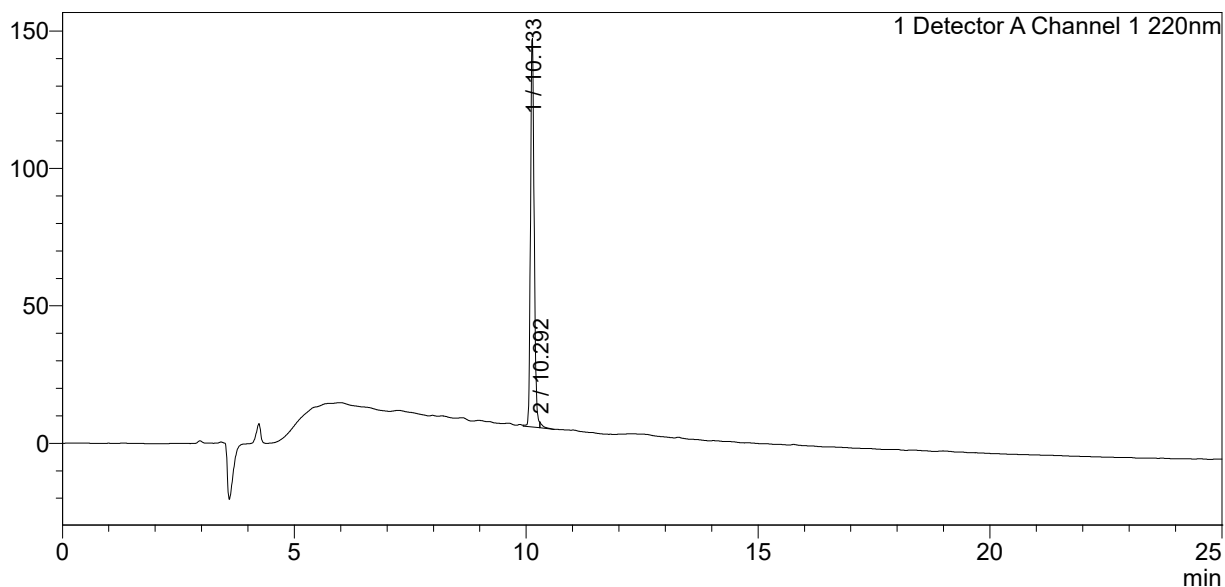

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.133	786408	141420	98.874
2	10.292	8954	2057	1.126
Total		795362	143476	100.000