

Sample Name :Substance P  
 Cat No. : RP10178  
 Lot No. : E5808725B  
 Time Processed :12:32:53  
 Month-Day-Year Processed :03/02/2025  
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ25010054

### <Chromatogram>

mV

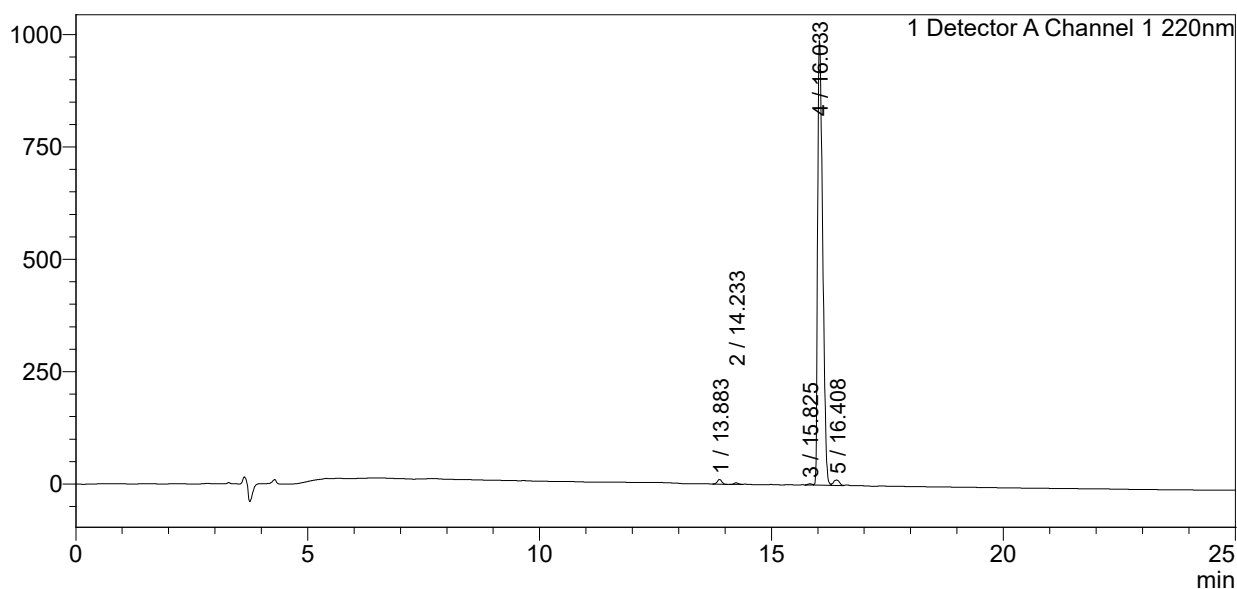

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.883	71601	10532	0.928
2	14.233	20468	3472	0.265
3	15.825	18579	2835	0.241
4	16.033	7501430	989558	97.173
5	16.408	107611	12092	1.394
Total		7719689	1018489	100.000