


Mass Spectrum

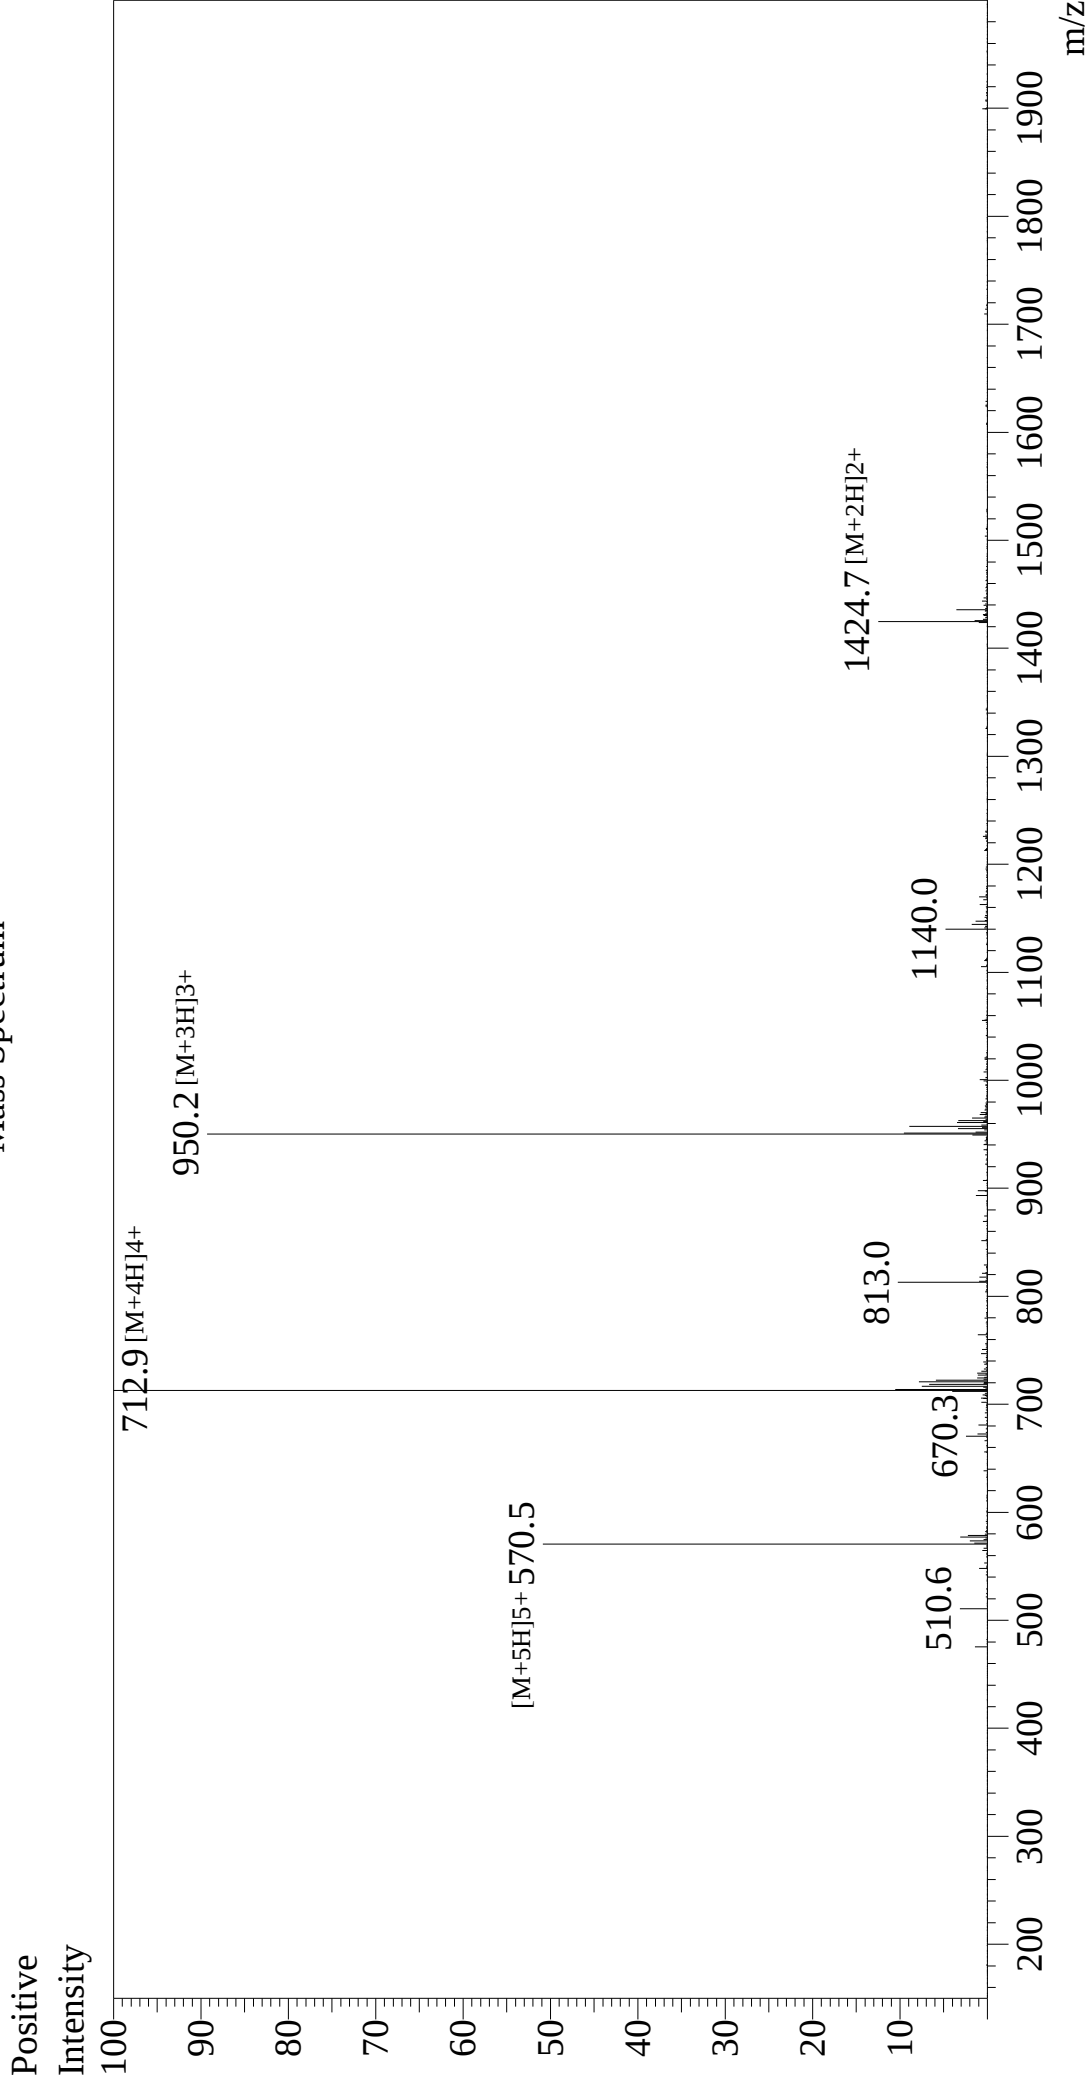

Sample Information

Month-Day Processed : 03/01/25
Time Processed : 2:54:06 PM
Injection Volume : 0.4
Sample Name : Melittin,honey bee

Cat No. : RP20415
Lot No. : E5809425B
Theoretical MW : 2847.50
Observed MW : 2847.6

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200
Equipment : ZJ22010150
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H₂O/50%MeOH