

Sample Name:Atrial Natriuretic Peptide (ANP) (1-28), human, porcine  
Cat No. : RP11927  
Lot No. : E5840623F  
Time Processed :10:08:28  
Month-Day-Year Processed :06/22/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ21010375

### <Chromatogram>

mV

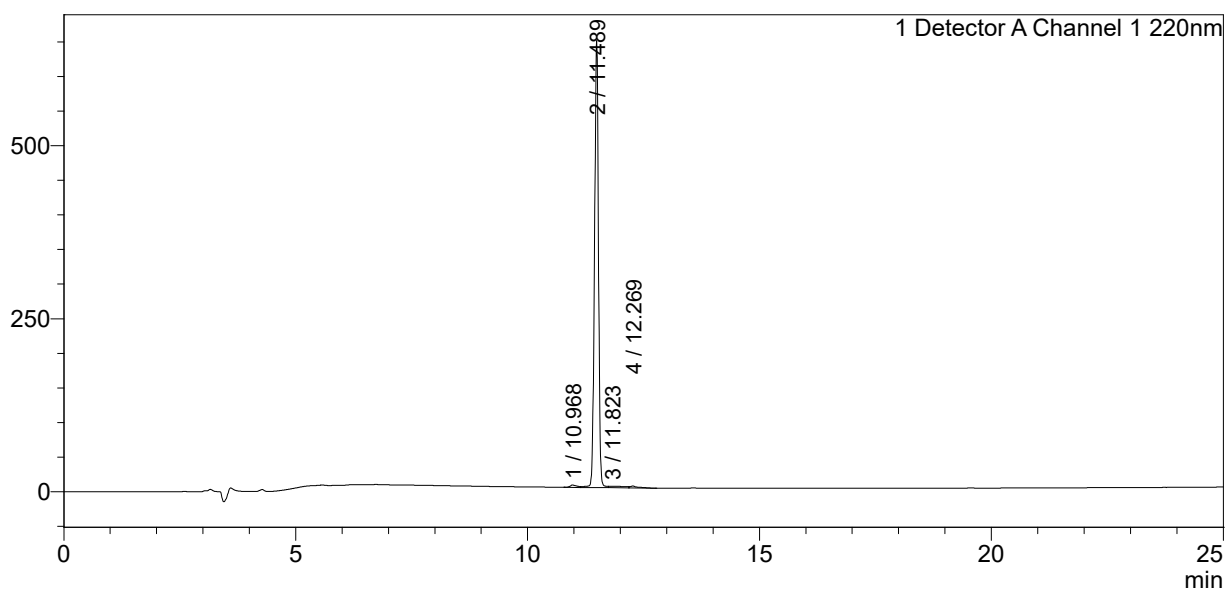

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.968	35210	3523	0.886
2	11.489	3851430	646166	96.937
3	11.823	53358	2263	1.343
4	12.269	33139	2778	0.834
Total		3973138	654730	100.000