

Sample Name : Calcitonin Gene Related Peptide (CGRP), rat
 Cat No. : RP11095
 Lot No. : E5930223I
 Time Processed : 9:05:16
 Month-Day-Year Processed : 09/09/2023

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm
 Equipment: ZJ17010507

<Chromatogram>

mV

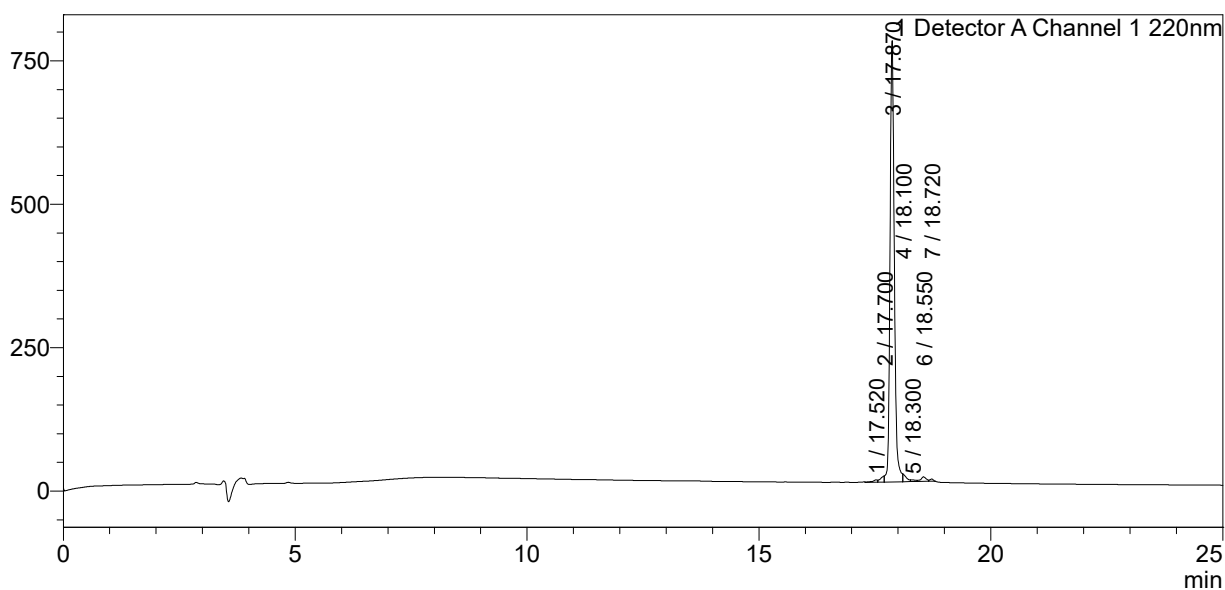

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.520	30160	3961	0.578
2	17.700	56943	10458	1.092
3	17.870	4957797	769345	95.054
4	18.100	71673	13451	1.374
5	18.300	19823	2680	0.380
6	18.550	61318	7913	1.176
7	18.720	18074	3554	0.347
Total		5215788	811360	100.000