


Mass Spectrum

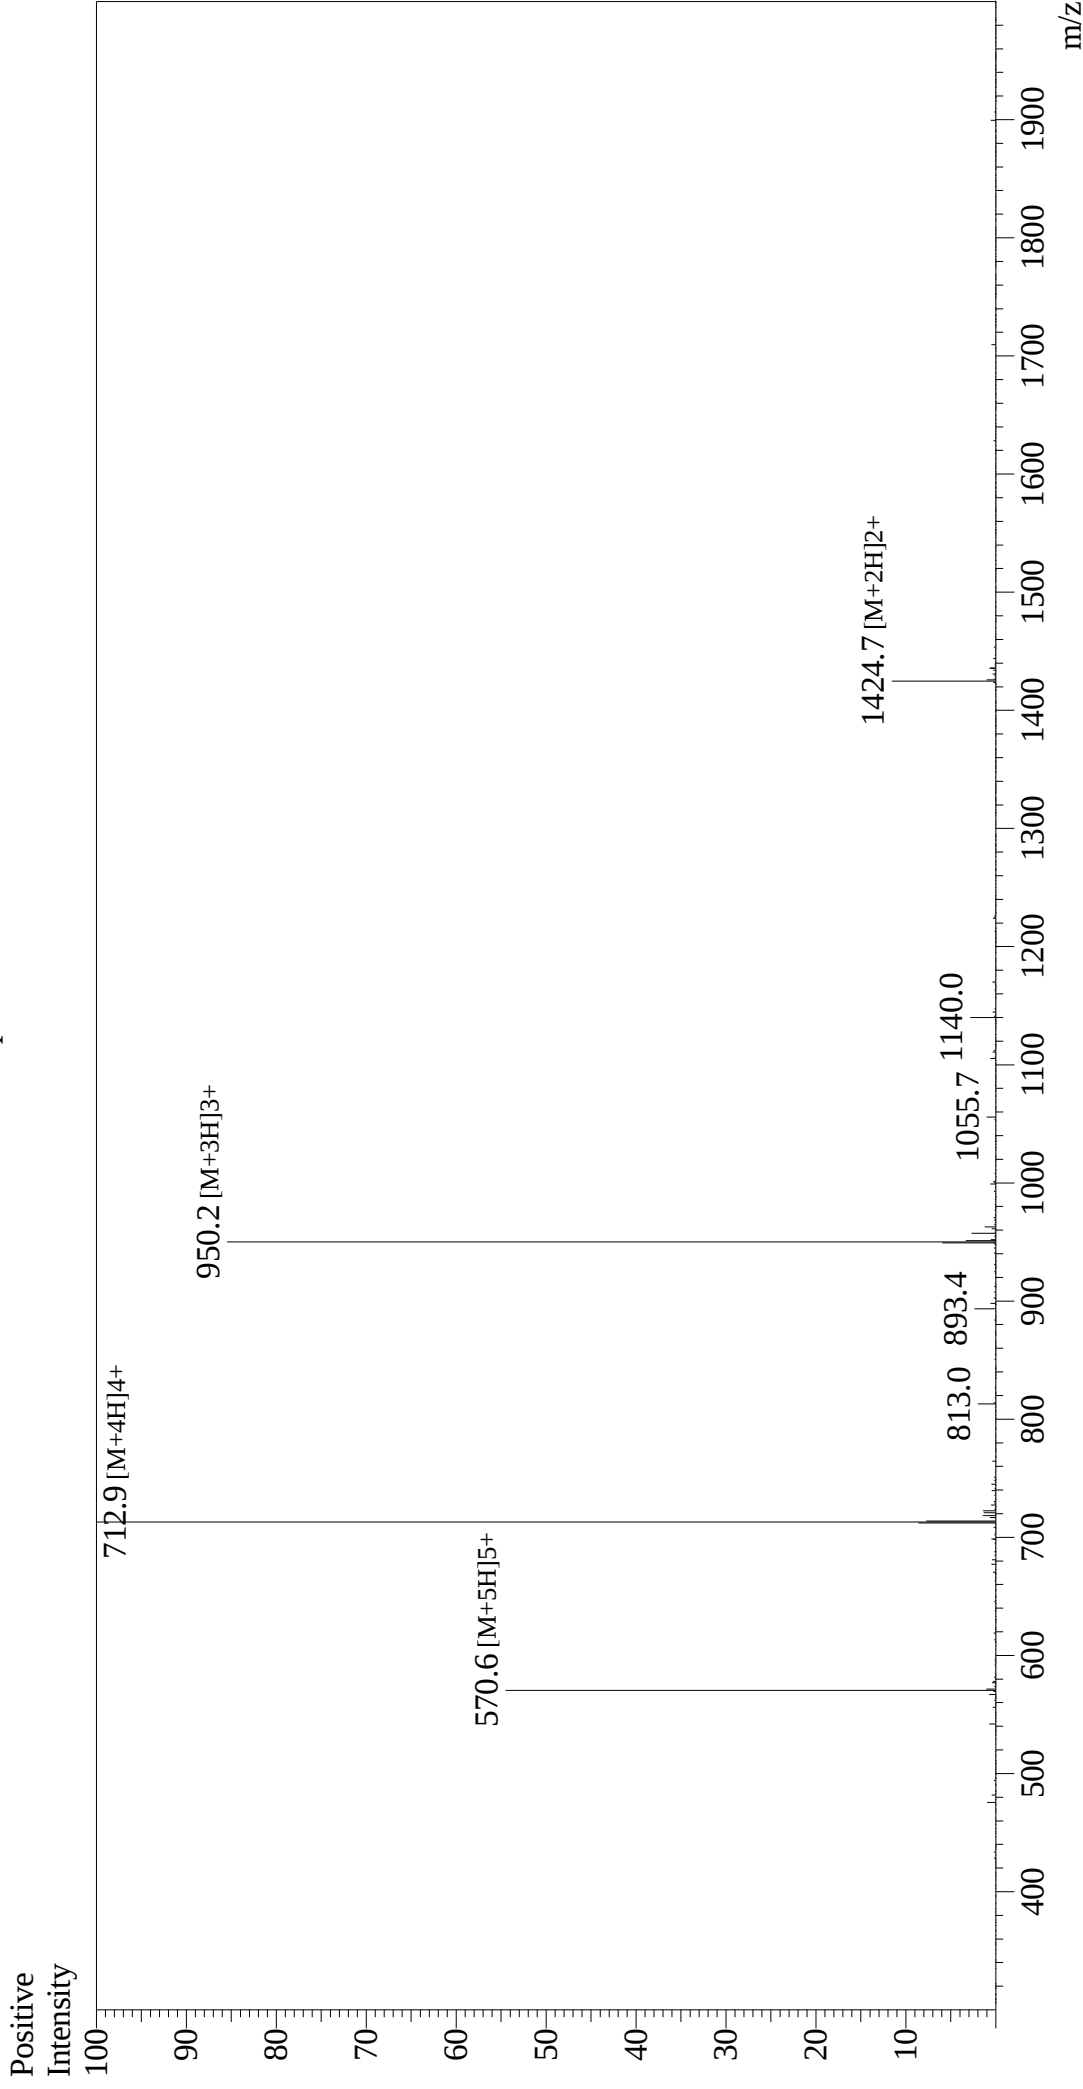

Sample Information

Month-Day Processed : 02/12/25
Time Processed : 15:21:15
Injection Volume : 0.4
Sample Name : Melittin,honey bee
Cat No. : RP20415
Lot No. : E5990425B
Theoretical MW: 2847.50
Observed MW : 2847.6

Interface :ESI

Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment : ZJ21010035

Interface Bias : +4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H₂O/50%MeOH