


Mass Spectrum

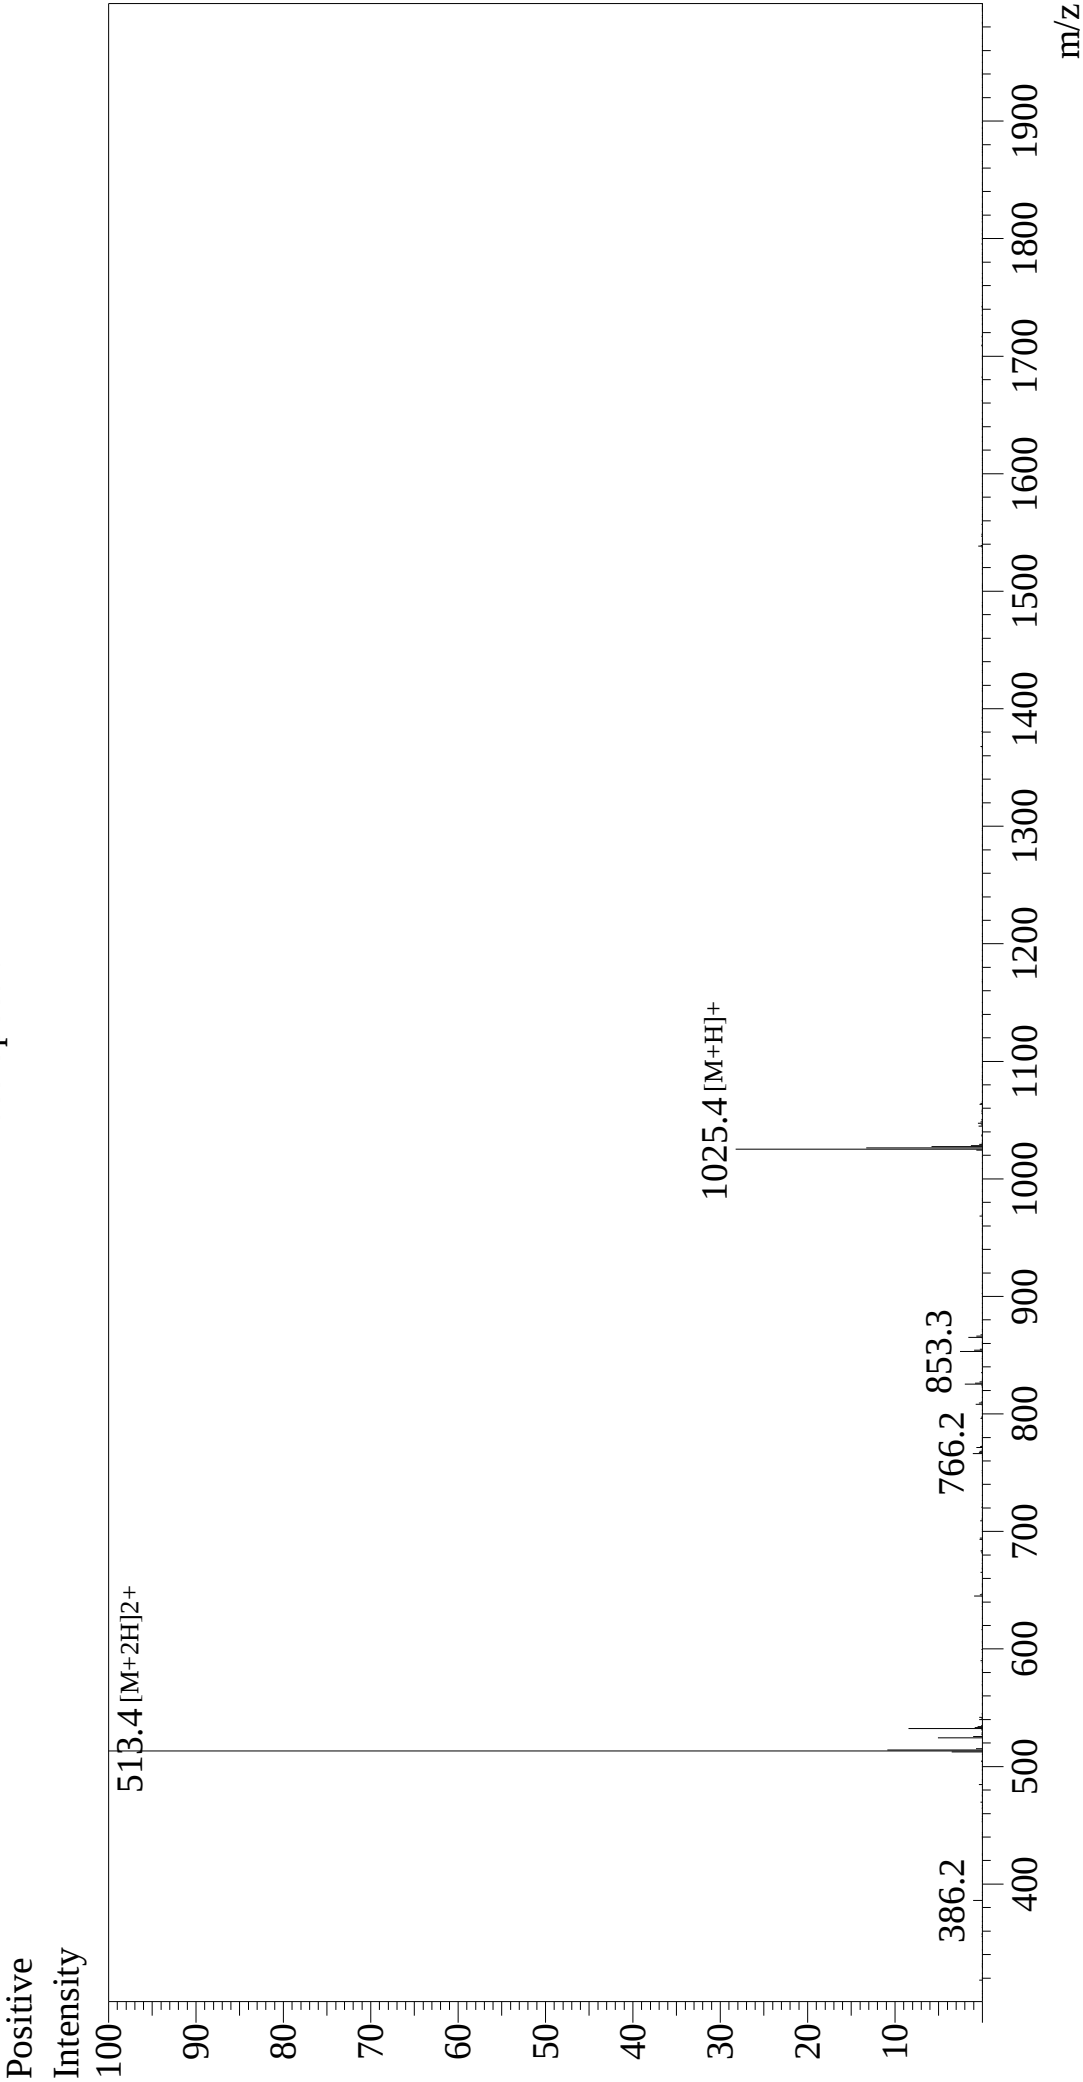

Sample Information		Equipment	
Month-Day Processed :	01/11/23	Interface	: ZJ21010035
Time Processed :	20:27:20	Nebulizing Gas Flow	: +4.5 kV
Injection Volume :	0.2	CDL Temp	: 5 L/min
Sample Name :	RGD	Drying Gas Flow	: 0.2 ml/min
Cat No. :	RP20297	Block Temp	: 50% H ₂ O/50% M
Lot No. :	E5996423A		
Theoretical MW: 1025.06			
Observed MW : 1024.8			