


Mass Spectrum

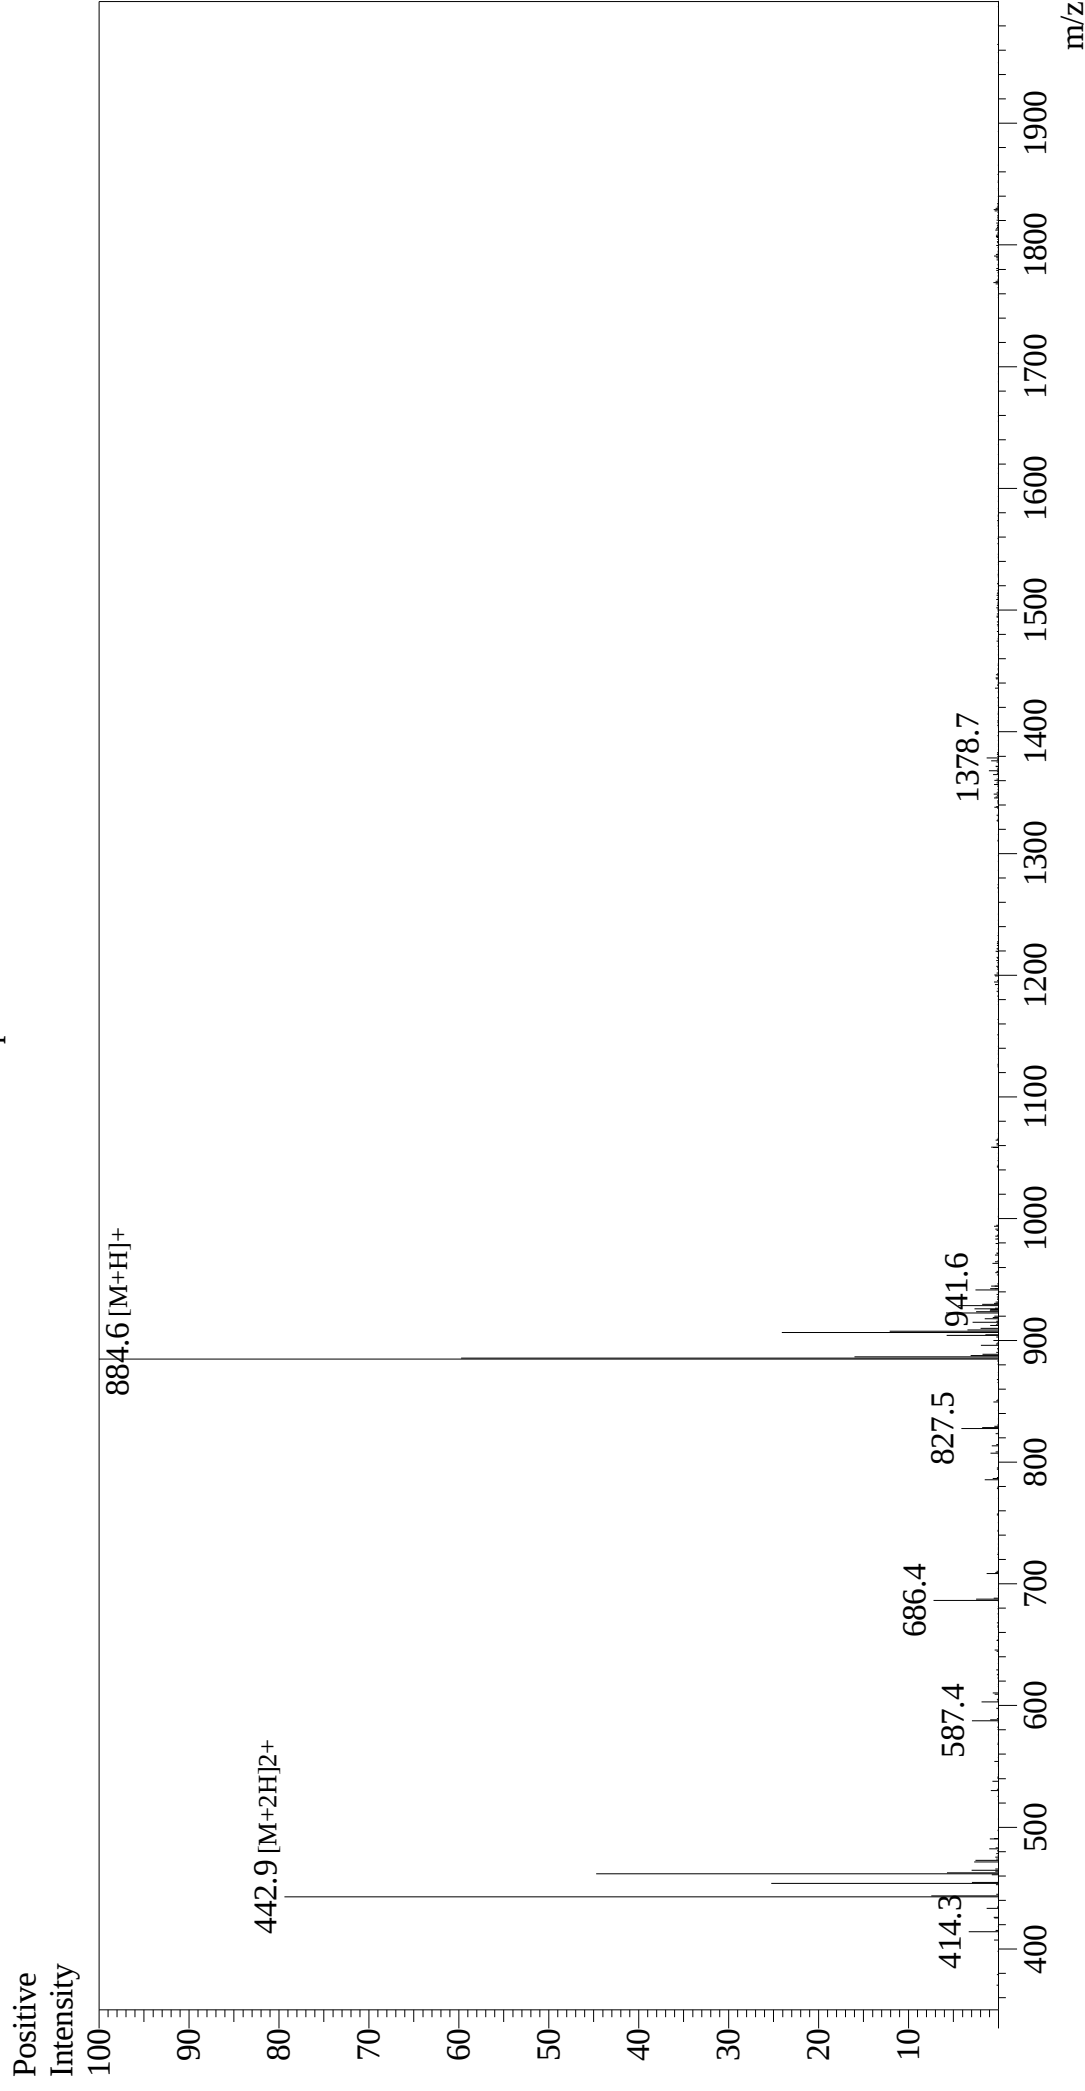

Sample Information

Month-Day Processed : 07/24/23
 Time Processed : 10:04:14
 Injection Volume : 0.3
 Sample Name : KRAS G12V Peptide (VVVGAVGVGK)
 Cat No. : RP30229
 Lot No. : E6078023G
 Theoretical MW : 884.08
 Observed MW : 883.6

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200

Equipment : ZJ21010035
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50%H2O/50%MeOH