

Sample Name :IRBP (1-20), human
 Cat No. : RP20269
 Lot No. : E6173625B
 Time Processed :22:37:25
 Month-Day-Year Processed :02/08/2025
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: ZJ19010142

<Chromatogram>

mV

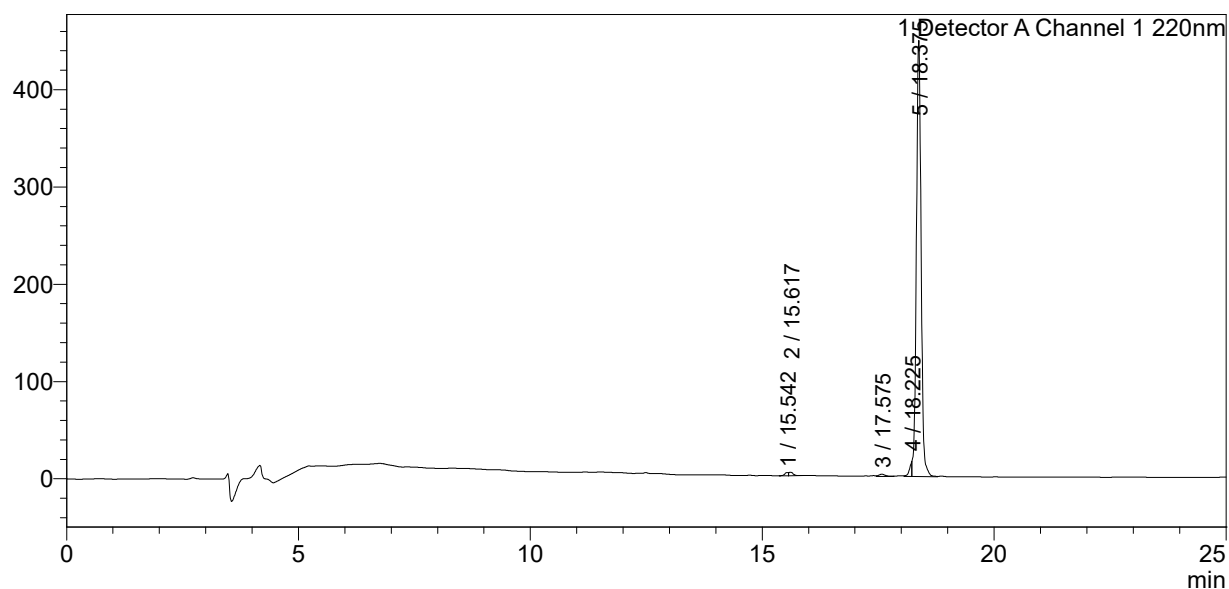

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.542	17036	3280	0.517
2	15.617	23101	3543	0.701
3	17.575	24002	2312	0.728
4	18.225	52456	15606	1.592
5	18.375	3178934	448532	96.462
Total		3295530	473272	100.000