

Sample Name: Calcitonin Gene Related Peptide (CGRP), rat
Cat No. : RP11095
Lot No. : E6275824D
Time Processed : 11:29:17
Month-Day-Year Processed : 05/24/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow: 1 ml/min
Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-SP 4.6 x 250 mm
Equipment: SS-CM-0309

<Chromatogram>

mV

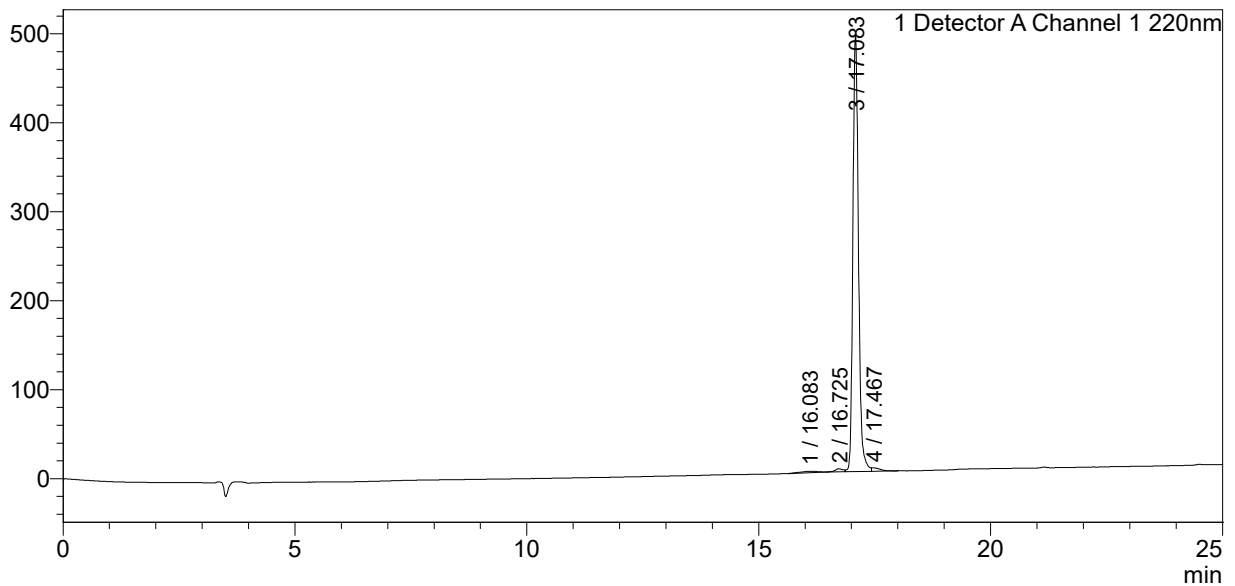

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.083	37045	1449	0.877
2	16.725	38911	3359	0.921
3	17.083	4100644	490066	97.089
4	17.467	47000	3764	1.113
Total		4223599	498639	100.000