


Mass Spectrum

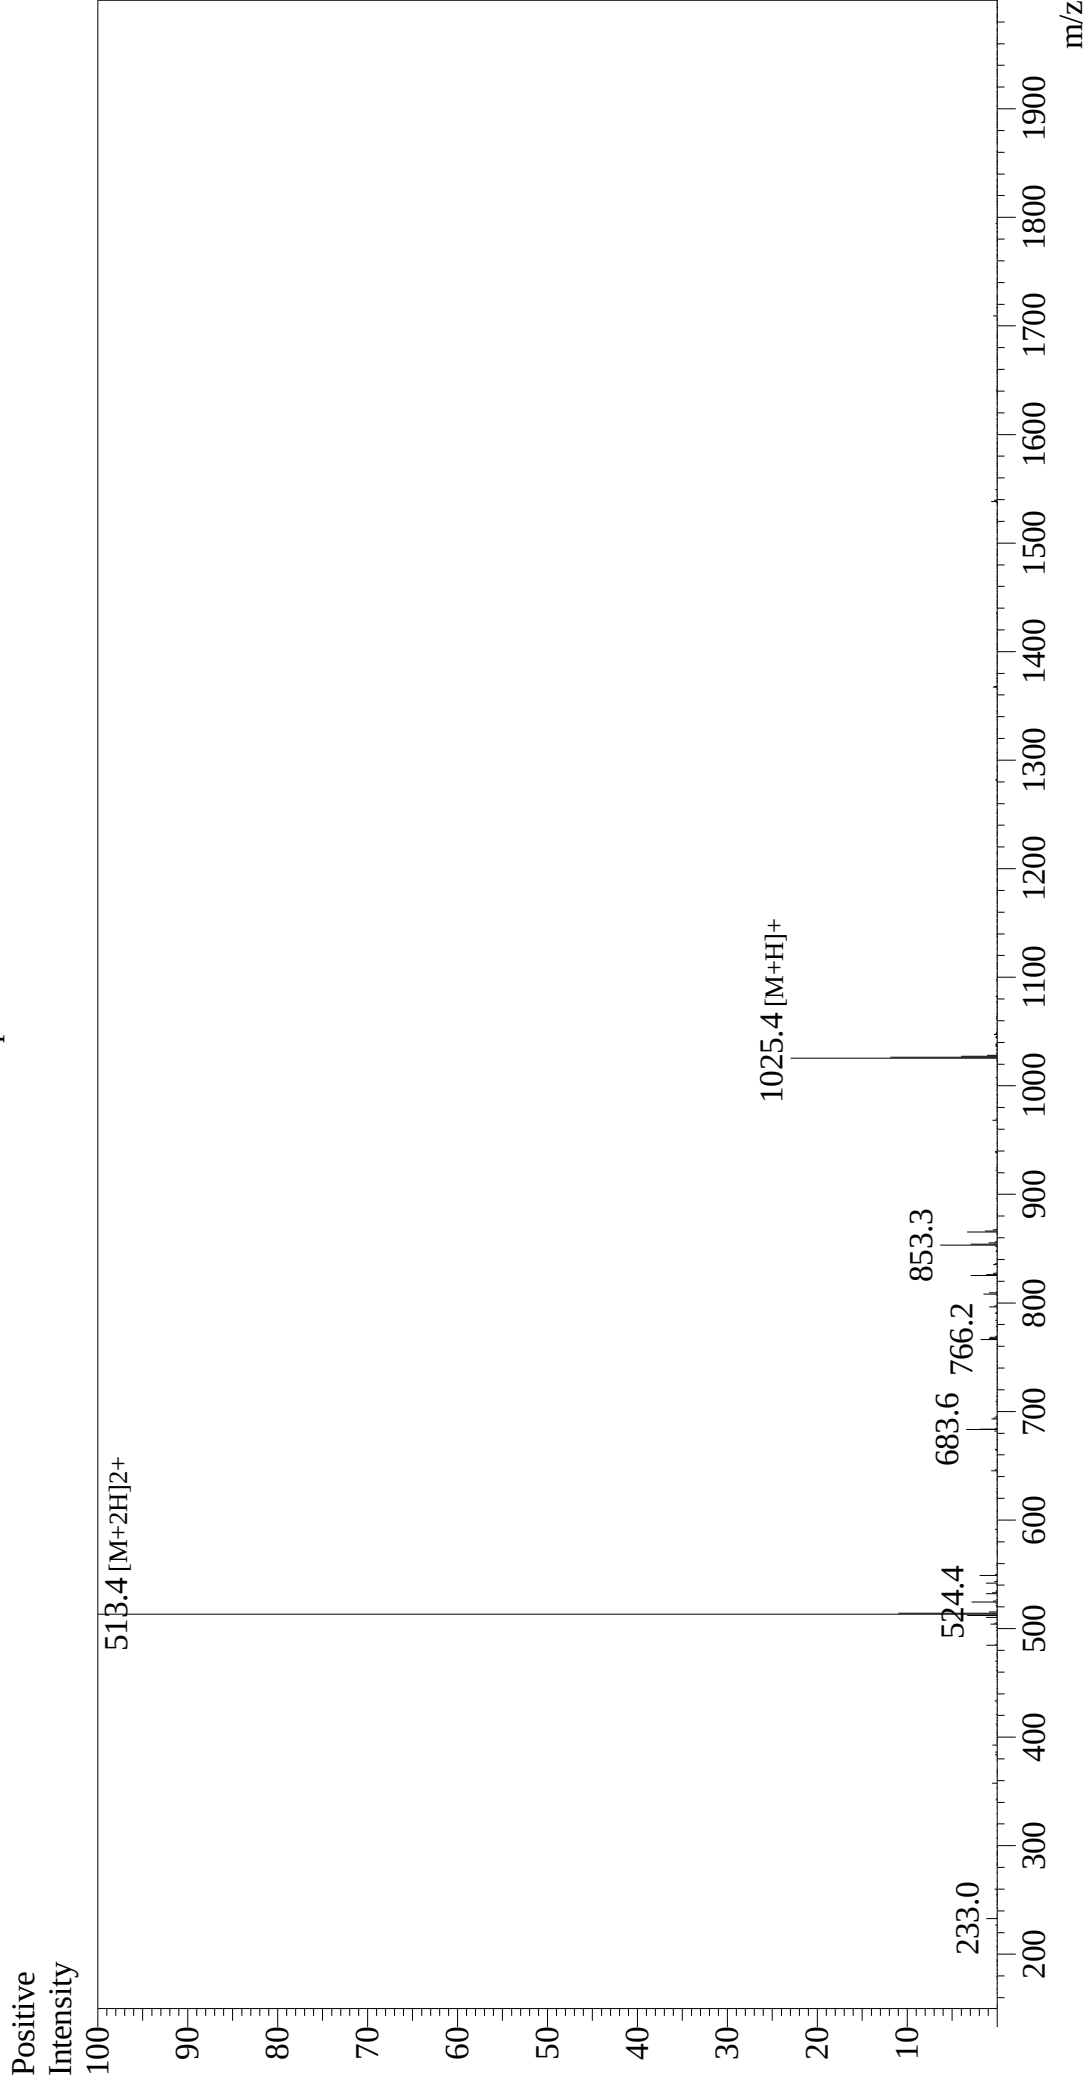

Sample Information

Month-Day Processed : 03/23/22
Time Processed : 8:31:53
Injection Volume : 0.2
Sample Name : RGD

Cat No. : RP20297
Lot No. : E6312622C
Theoretical MW:1025.06
Observed MW :1024.8

Interface :ESI
Nebulizing Gas Flow :1.5L/min
CDL Temp :250
Block Temp :200

Equipment : ZJ21010035
Interface Bias : +4.5 kV
Drying Gas Flow :5 L/min
T.Flow :0.2 ml/min
B.conc :50%H₂O/50%MeOH