

Sample Name :Substance P
Cat No. : RP10178
Lot No. : E6420124A
Time Processed :17:50:52
Month-Day-Year Processed :01/25/2024

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm

Equipment: GR11010440

<Chromatogram>

mV

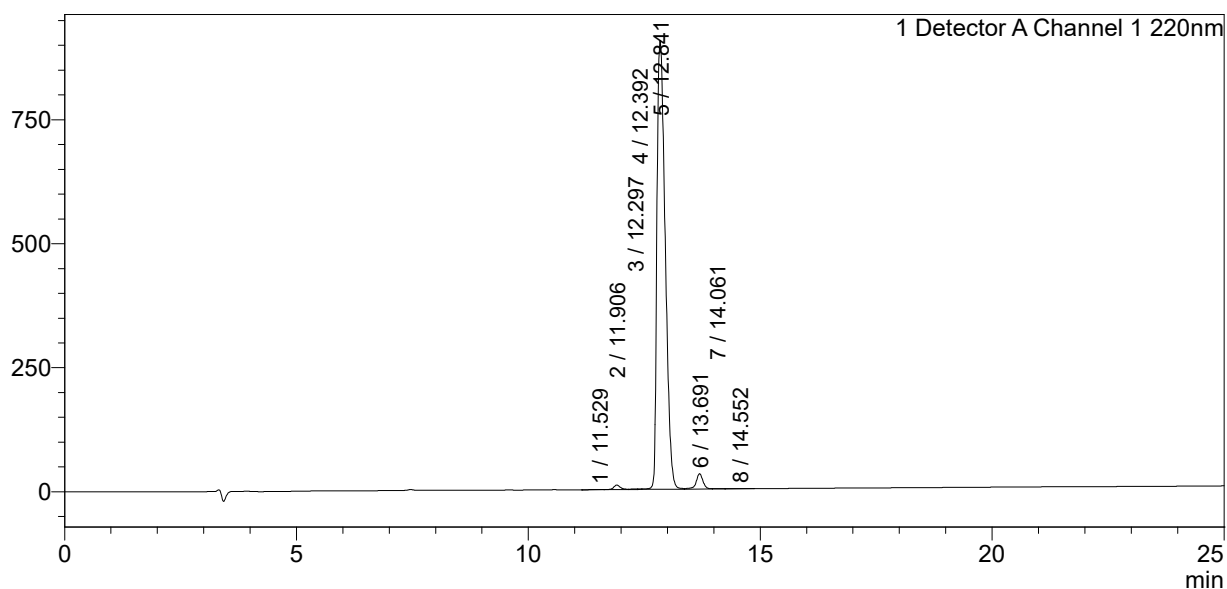

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.529	4241	327	0.036
2	11.906	94442	9148	0.807
3	12.297	10675	1098	0.091
4	12.392	5261	968	0.045
5	12.841	11254388	905164	96.202
6	13.691	316575	31032	2.706
7	14.061	4812	380	0.041
8	14.552	8331	345	0.071
Total		11698726	948462	100.000